

Sample Name : Iα52
 Cat. No. : RP20228
 Lot. No. : E4851319I
 Time Processed : 13:00:14
 Month-Day-Year Processed : 09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.00	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010009

Chromatogram

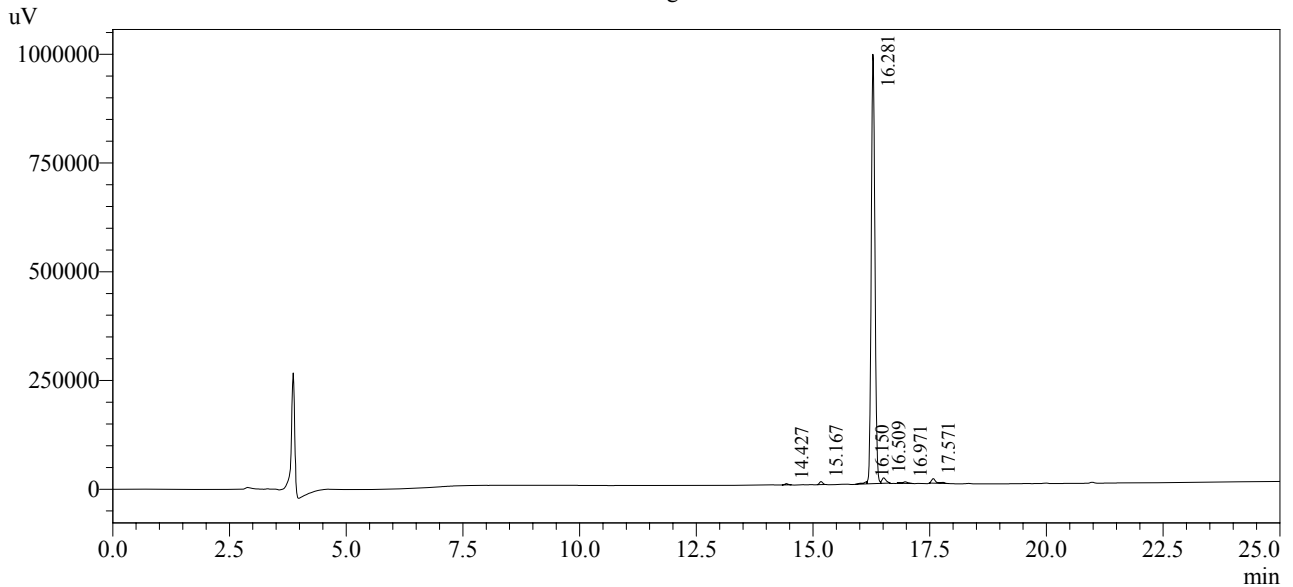

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.427	13389	2898	0.236
2	15.167	33125	6702	0.584
3	16.150	34911	5040	0.616
4	16.281	5405727	987316	95.366
5	16.509	75070	12452	1.324
6	16.971	29891	3606	0.527
7	17.571	76260	10425	1.345
Total		5668373	1028440	100.000