

Sample Name : [Arg8]-Vasotocin
 Cat No.: RP10061
 Lot No.:E3607219K
 Time Processed :15:33:42
 Month-Day-Year Processed :11/13/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

mV

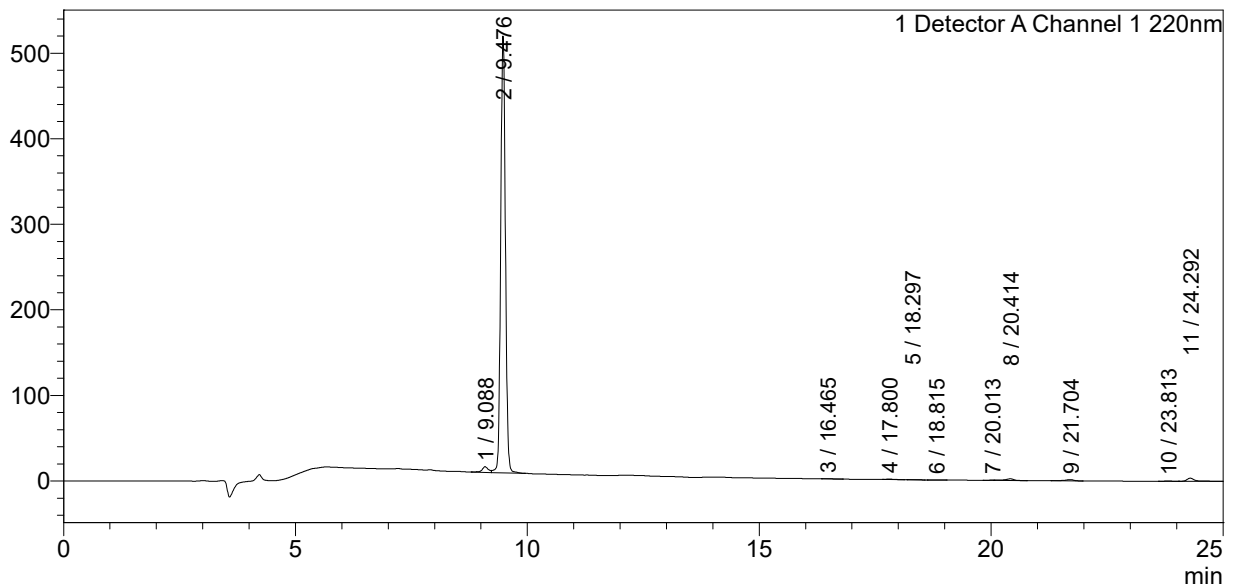

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.088	65196	6725	1.719
2	9.476	3625250	510654	95.582
3	16.465	3338	265	0.088
4	17.800	5513	575	0.145
5	18.297	2278	144	0.060
6	18.815	1321	123	0.035
7	20.013	1432	173	0.038
8	20.414	25905	1954	0.683
9	21.704	18855	1440	0.497
10	23.813	3338	236	0.088
11	24.292	40379	3589	1.065
Total		3792805	525878	100.000