

Sample Name :  $\beta$ -Melanocyte Stimulating Hormone (MSH), human  
 Cat No.: RP10648  
 Lot No.:E7561820B  
 Time Processed :17:08:03  
 Month-Day-Year Processed :02/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>  
 Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment:ZJ19010324

<Chromatogram>

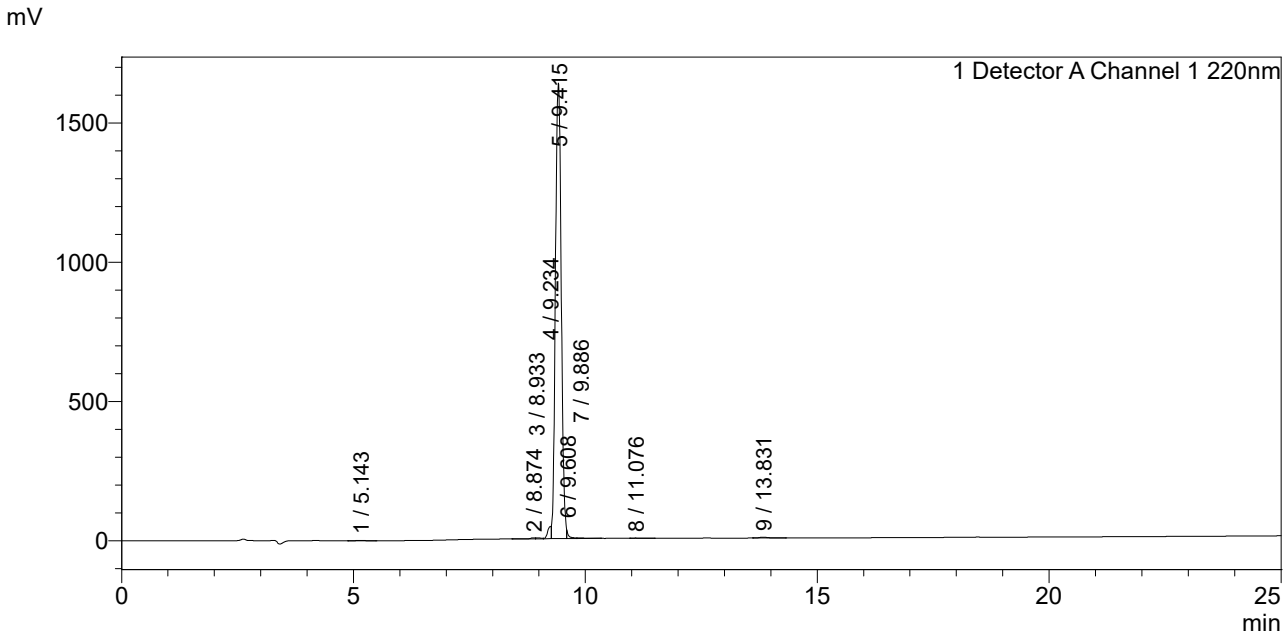

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.143	9779	1155	0.066
2	8.874	23911	3766	0.162
3	8.933	24087	2821	0.163
4	9.234	243843	43377	1.653
5	9.415	14297523	1636761	96.908
6	9.608	80904	24014	0.548
7	9.886	30244	2666	0.205
8	11.076	6437	809	0.044
9	13.831	36995	3067	0.251
Total		14753723	1718436	100.000