

Sample Name:Neurotensin
 Cat No :RP10439
 Lot No :E4756721D
 Time Processed :17:46:51
 Month-Day-Year Processed :04/24/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

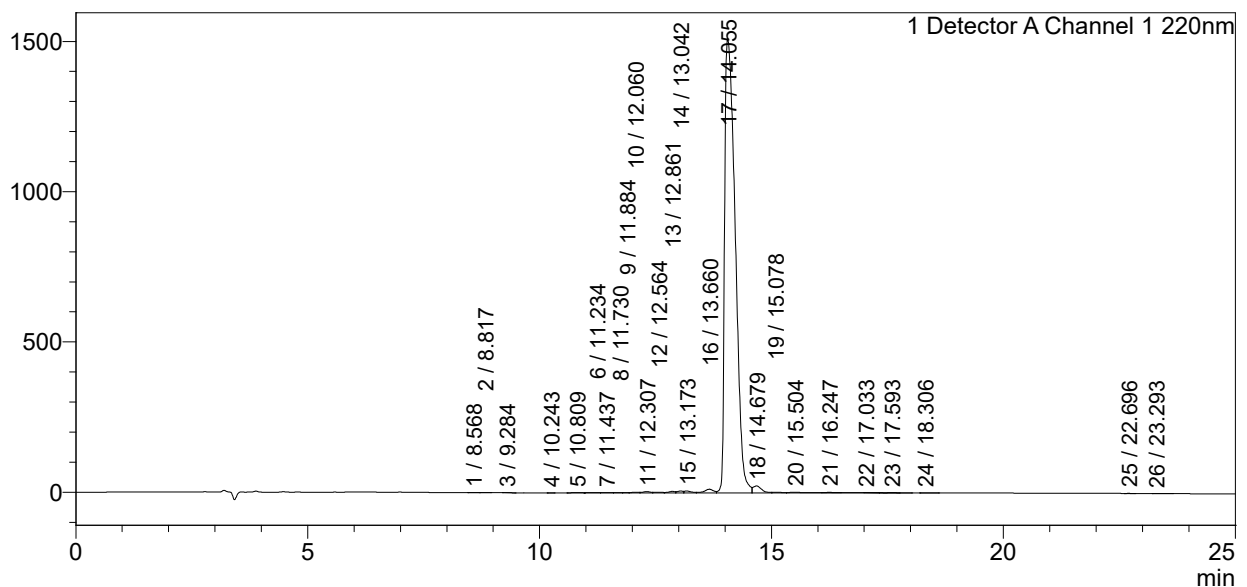

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.568	3415	507	0.014
2	8.817	2754	437	0.011
3	9.284	1230	146	0.005
4	10.243	1048	160	0.004
5	10.809	6166	447	0.025
6	11.234	6473	466	0.026
7	11.437	8148	607	0.033
8	11.730	7918	808	0.032
9	11.884	7116	918	0.029
10	12.060	21307	2028	0.086
11	12.307	45570	4317	0.183
12	12.564	28057	2303	0.113
13	12.861	48059	4873	0.193
14	13.042	51302	5850	0.206
15	13.173	63831	5992	0.257
16	13.660	161907	11990	0.651

Peak#	Ret. Time	Area	Height	Area%
17	14.055	23985659	1511574	96.411
18	14.679	287867	22817	1.157
19	15.078	27992	1817	0.113
20	15.504	89882	2123	0.361
21	16.247	10333	1335	0.042
22	17.033	1919	126	0.008
23	17.593	5653	662	0.023
24	18.306	1464	111	0.006
25	22.696	1207	165	0.005
26	23.293	2200	121	0.009
Total		24878476	1582699	100.000