

Sample Name :Carcinoembryonic Antigen (CEA)
 Cat No :RP20328
 Lot No :E2541420J
 Time Processed :13:09:18
 Month-Day-Year Processed :10/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

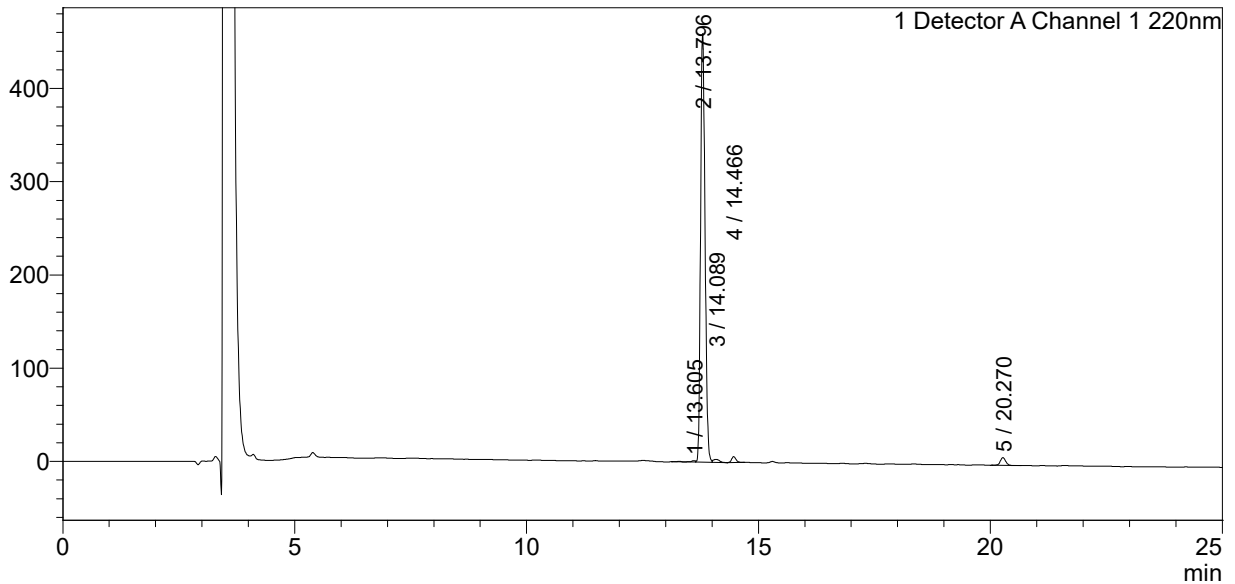

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.605	11191	1474	0.347
2	13.796	3079966	459730	95.392
3	14.089	29145	3256	0.903
4	14.466	41441	6299	1.284
5	20.270	67013	8331	2.076
Total		3228756	479091	100.000