

Sample Name :EGFRvIII peptide (PEPvIII)
 Cat. No. : RP20356
 Lot. No. : F6895220H
 Time Processed: 8:25:27

Month-Day-Year Processed :08/15/2020
 Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010324

<Chromatogram>

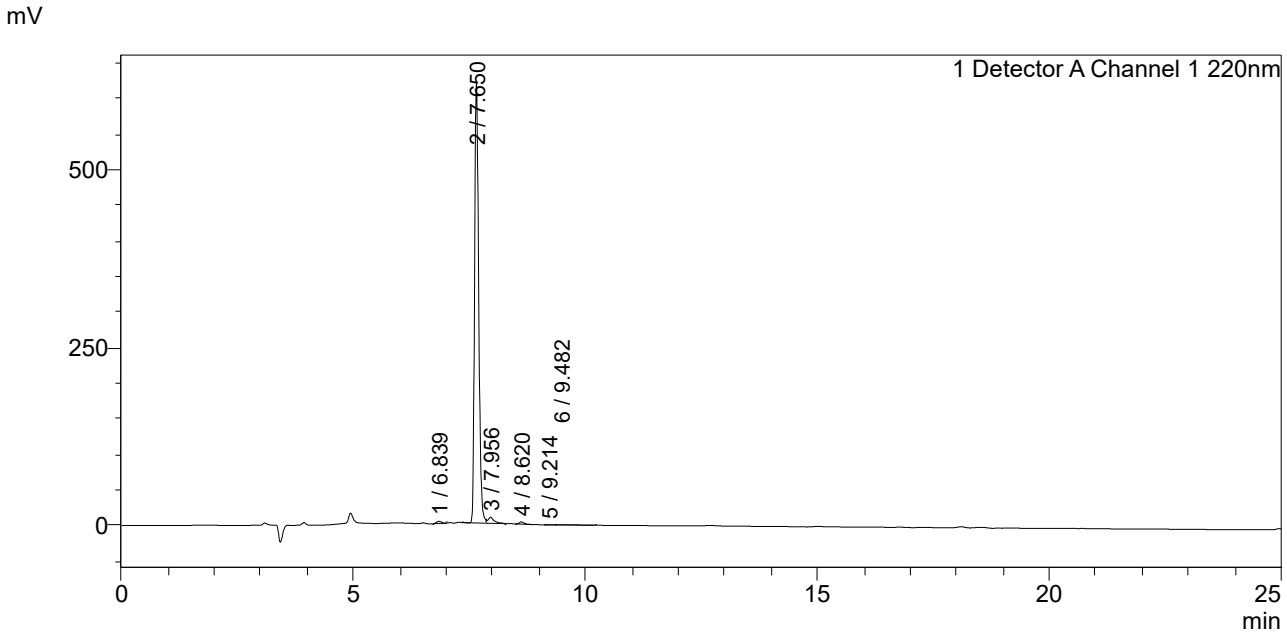

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.839	22254	2922	0.565
2	7.650	3819852	620526	96.901
3	7.956	71985	8618	1.826
4	8.620	19949	3002	0.506
5	9.214	1164	155	0.030
6	9.482	6802	199	0.173
Total		3942004	635422	100.000