


Mass Spectrum

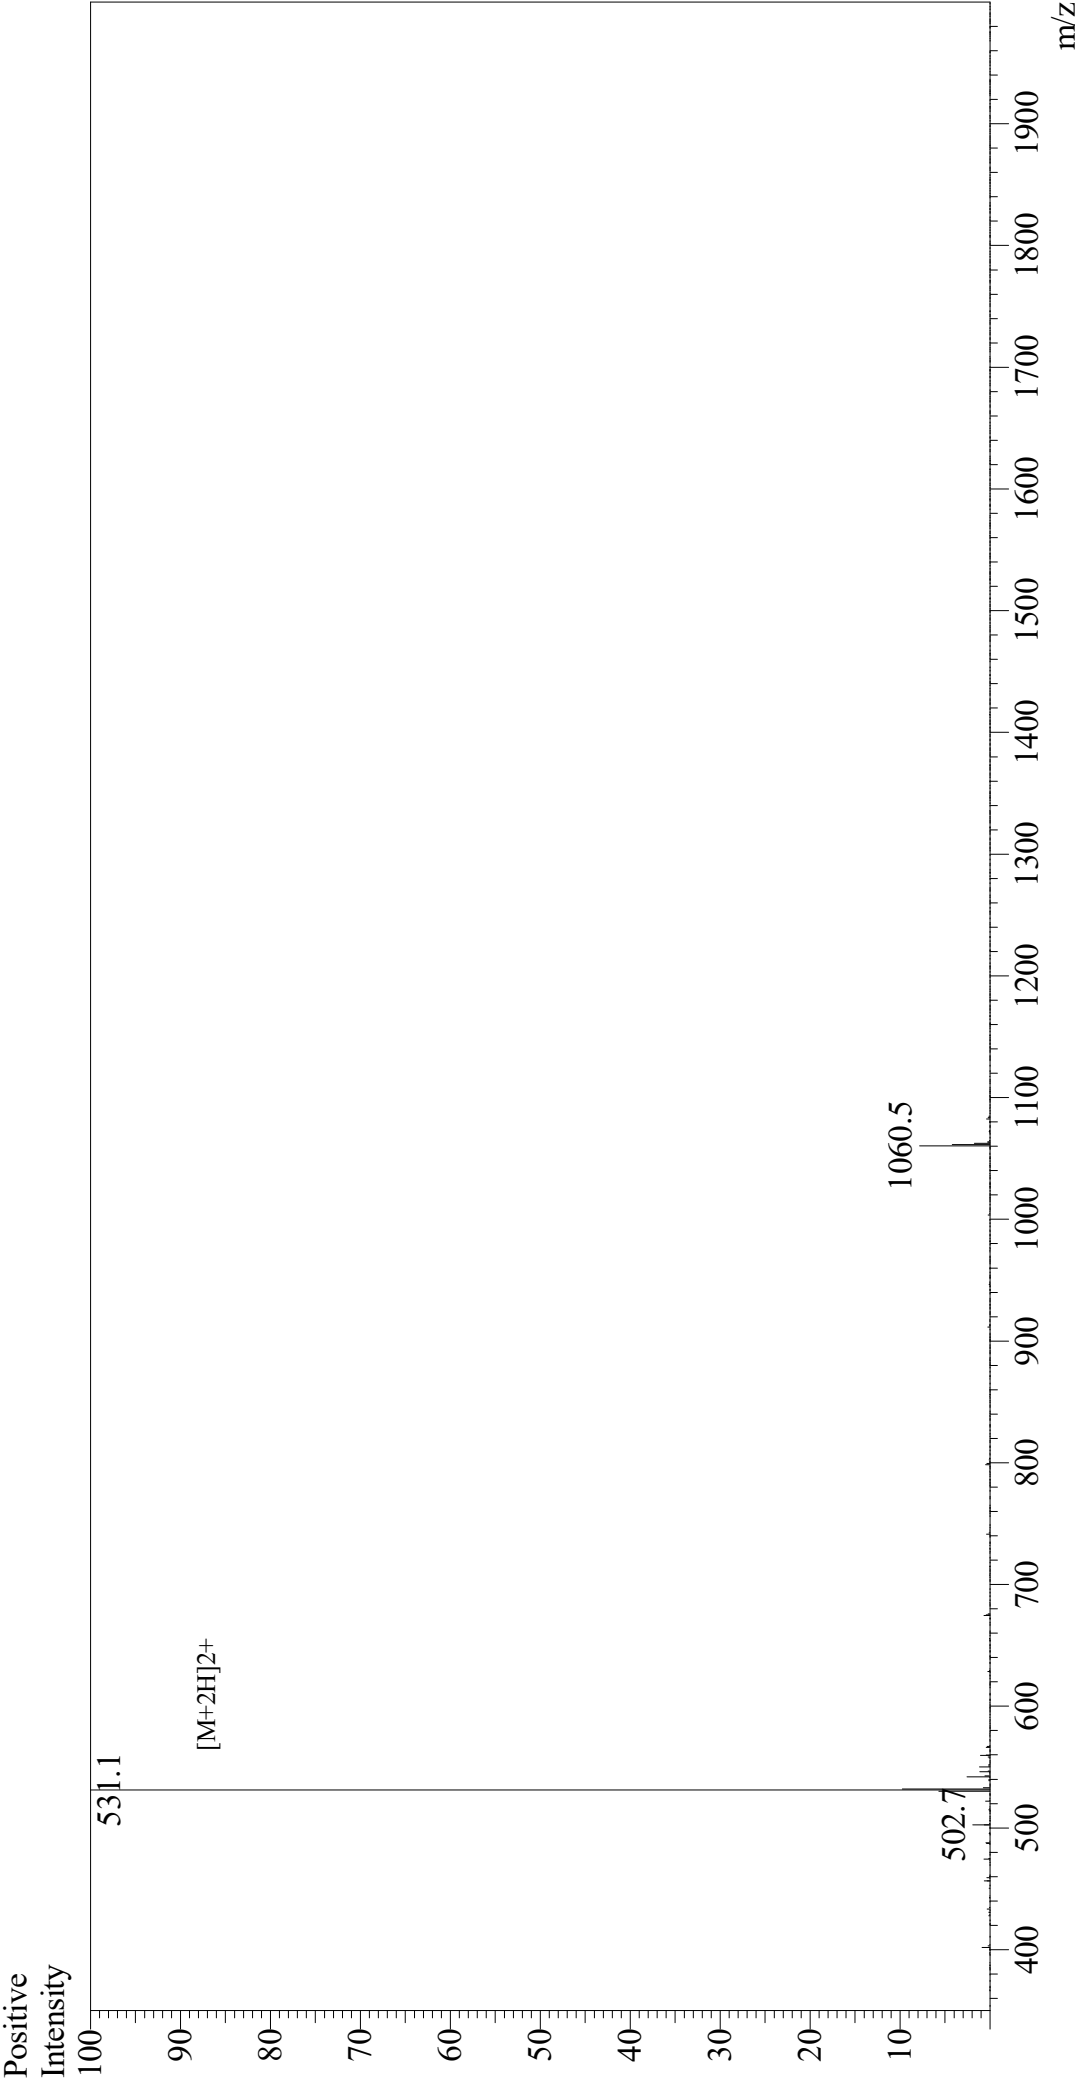

Sample Information

Month-Day Processed :	11/17/21	Equipment	: ZJ21010035
Time Processed :	11:24:58	Interface Bias	: +4.5 kV
Injection Volume :	0.2	Drying Gas Flow	: 5 L/min
Sample Name :	β-Amyloid (25-35)	T.Flow	: 0.2 ml/min
Cat No. :	RP10008	B.conc	: 50% H ₂ O/50% MeOH
Lot No. :	E9213021J		
Theoretical MW :	1060.27		
Observed MW :	1060.2		