

Sample Name :Influenza HA (518-526)  
 Cat. No. :RP20284  
 Lot. No. :PE2441810  
 Time Processed : 7:23:46  
 Month-Day-Year Processed : 10/10/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	15	
25.00	Pumps	Pump A B.Conc	75	
25.01	Pumps	Pump A B.Conc	95	
30.00	Pumps	Pump A B.Conc	95	
30.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: G09010878

Chromatogram

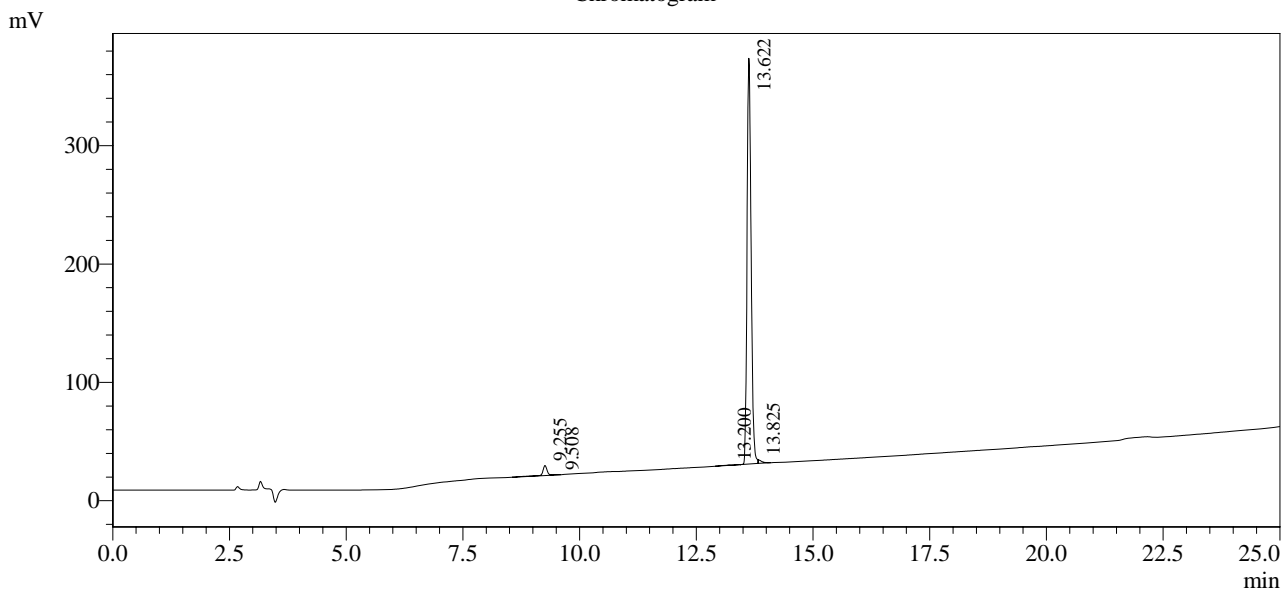

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.255	57887	8486	2.693
2	9.508	1638	152	0.076
3	13.200	5249	378	0.244
4	13.622	2069135	342939	96.272
5	13.825	15349	3129	0.714
Total		2149257	355084	100.000