

Sample Name :CDK5 Substrate (Phospho-Thr3)
 Cat No :RP20107
 Lot No :E2973920L
 Time Processed :1:25:39
 Month-Day-Year Processed :12/31/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
31.00	Pumps	B.Conc	95
31.01	Pumps	B.Conc	5
40.00	Pumps	B.Conc	5
40.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010140

<Chromatogram>

mV

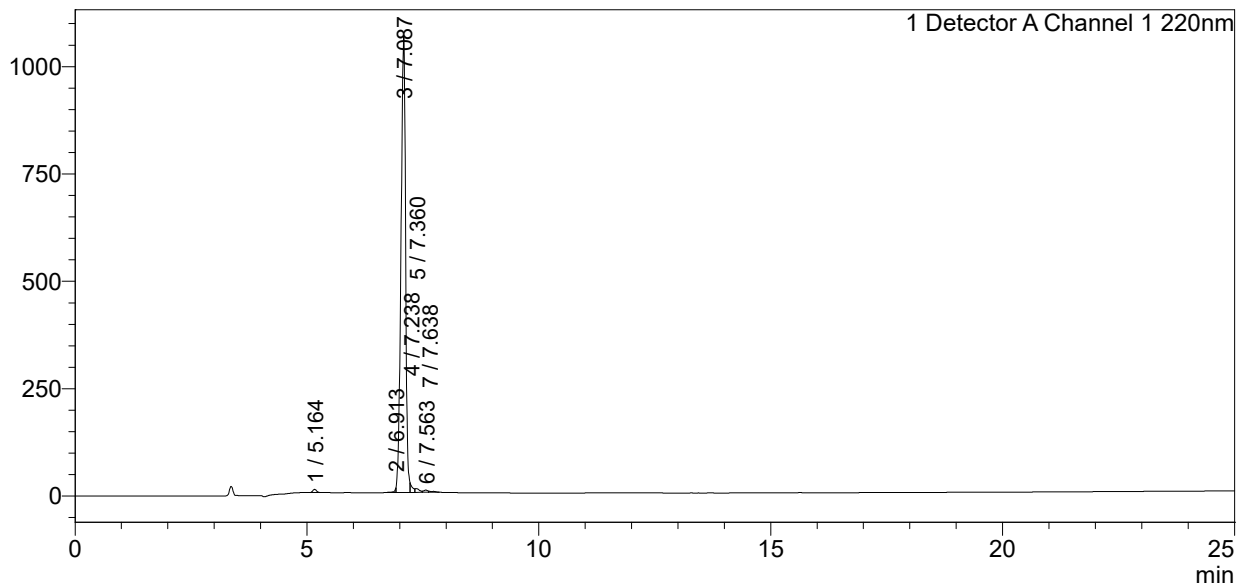

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.164	39443	7277	0.521
2	6.913	24150	7126	0.319
3	7.087	7326337	1063804	96.828
4	7.238	70781	19214	0.935
5	7.360	56091	8660	0.741
6	7.563	32100	5071	0.424
7	7.638	17453	2239	0.231
Total		7566355	1113391	100.000