

Sample Name :LSKL, Inhibitor of Thrombospondin (TSP-1)
 Cat. No. :RP19990
 Lot. No. :E1187919F
 Time Processed : 7:48:45
 Month-Day-Year Processed :06/20/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

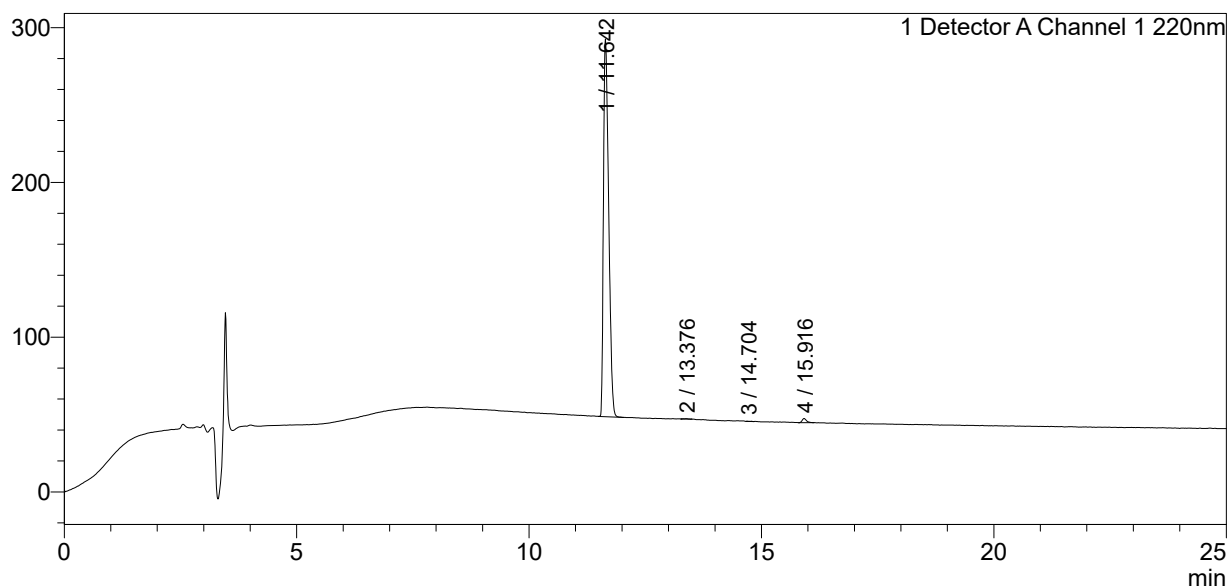

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.642	1897490	243978	98.963
2	13.376	1671	279	0.087
3	14.704	1101	188	0.057
4	15.916	17119	2713	0.893
Total		1917381	247159	100.000