

Sample Name :Angiotensin I, human
 Cat No. : RP11251
 Lot No. : E6378220B
 Time Processed :10:24:08
 Month-Day-Year Processed :02/16/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : AlltimaTM C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

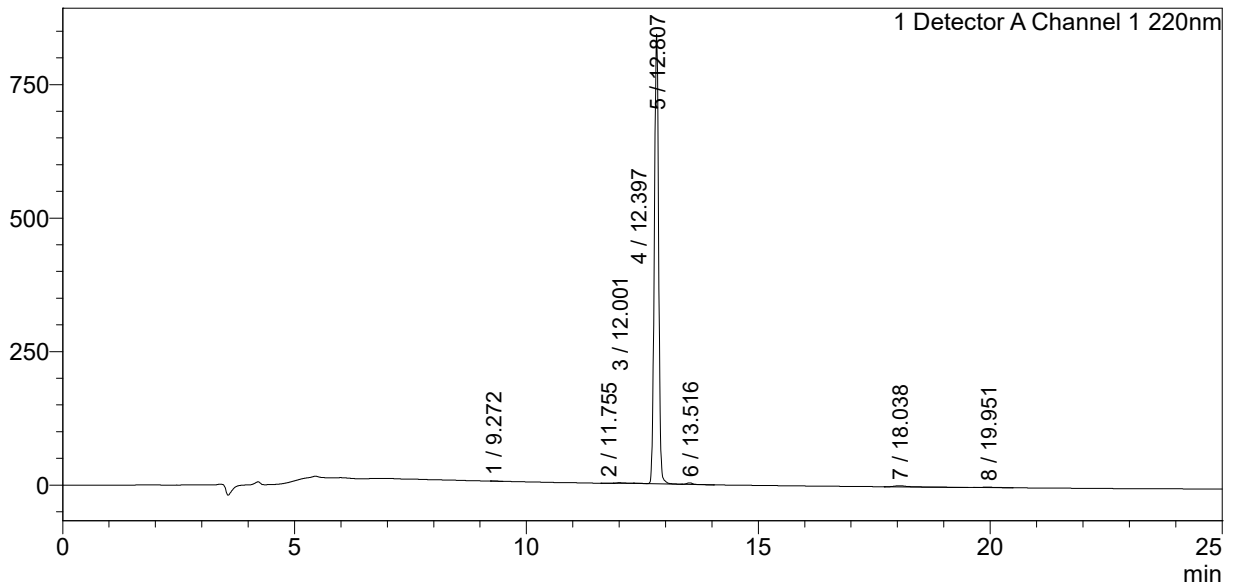

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.272	1026	104	0.018
2	11.755	1063	125	0.019
3	12.001	10880	1100	0.195
4	12.397	3269	330	0.059
5	12.807	5456540	842584	97.854
6	13.516	30157	3088	0.541
7	18.038	55225	2285	0.990
8	19.951	18058	823	0.324
Total		5576218	850440	100.000