


Mass Spectrum

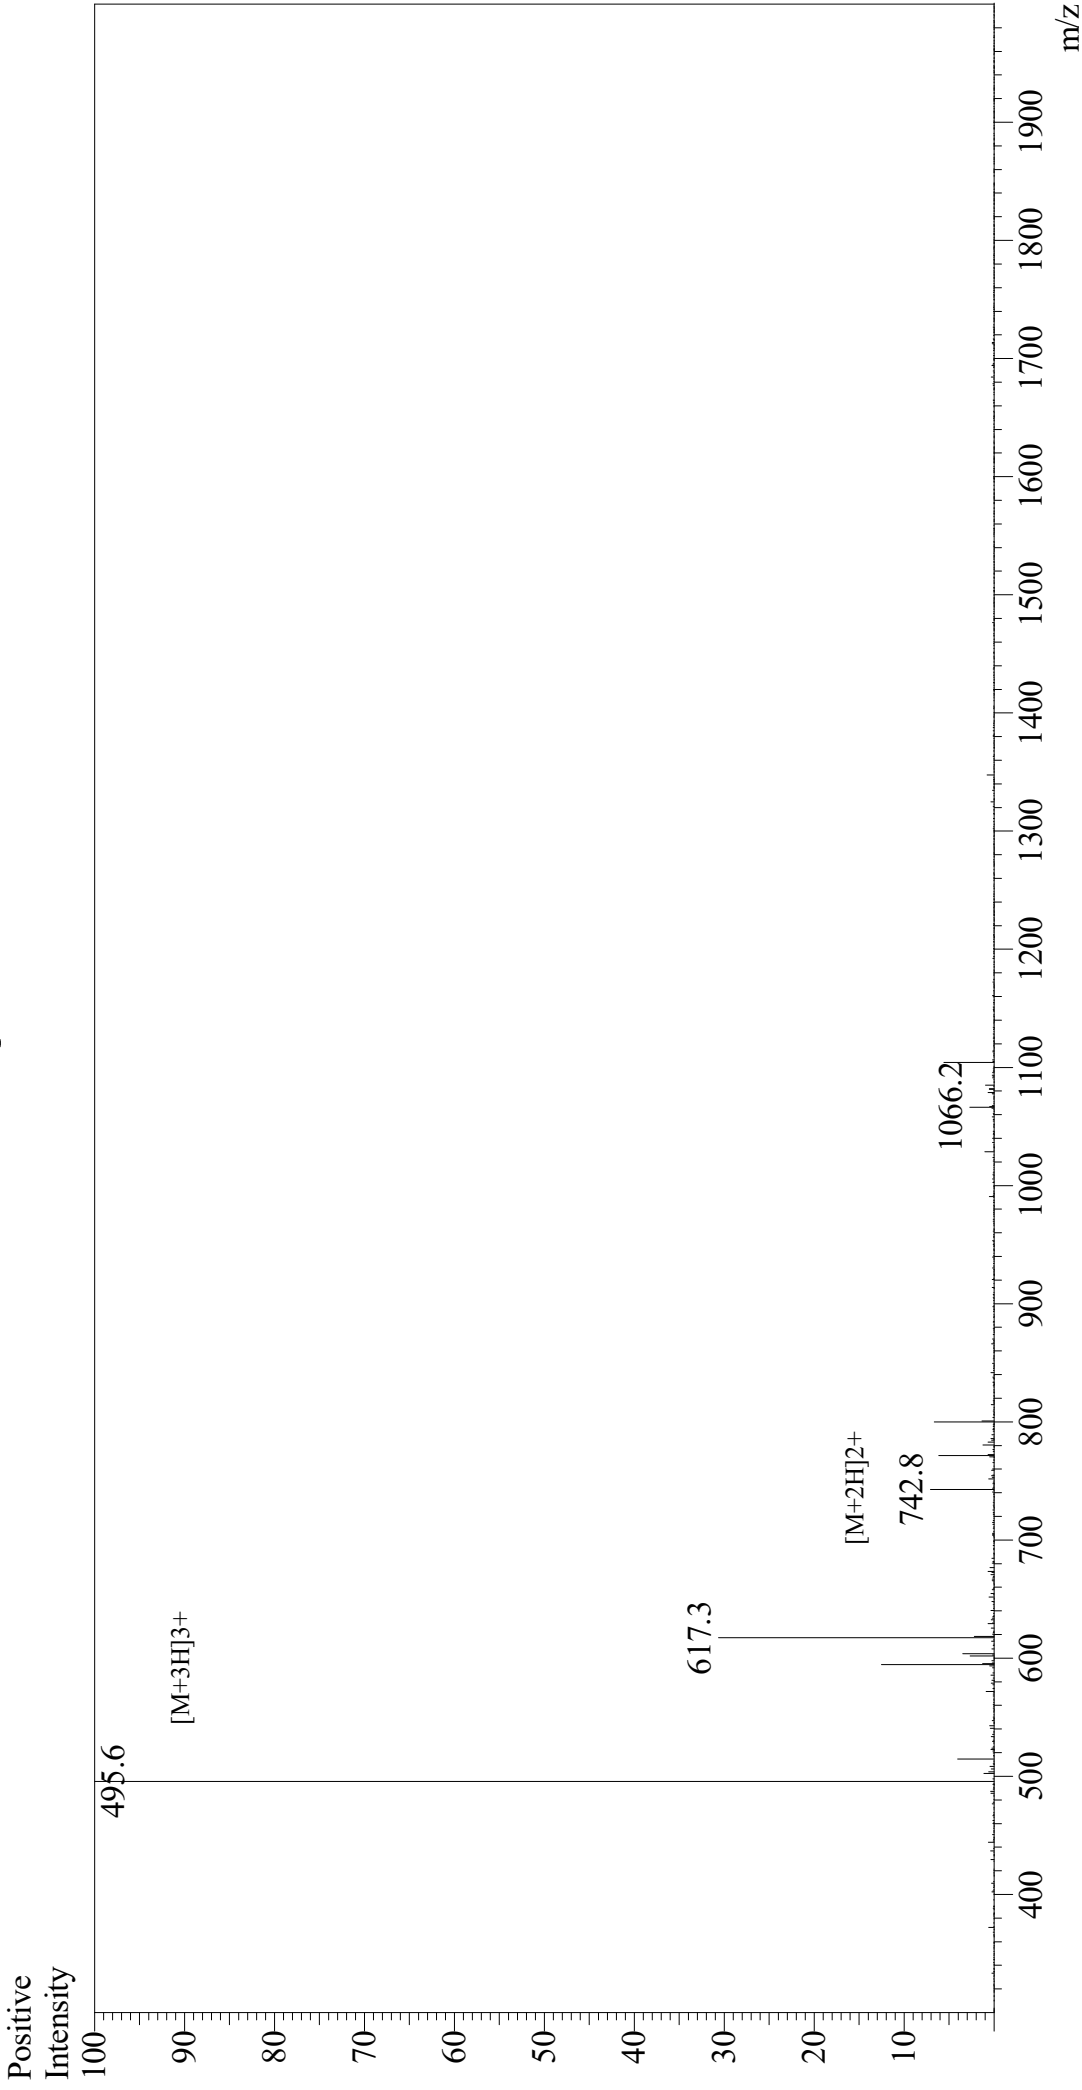

Sample Information

Acquired by: Gary
Month-Day Processed: 10/08/19
Time Processed: 03:03:19 PM
Injection Volume: 0.4
Sample Name: Bactenecin, bovine
Cat. No.: RP11235
Lot. No.: E4782919I
Theoretical MW: 1483.90
Observed MW: 1483.8

Interface: ESI
Nebulizing Gas Flow: 1.5L/min
CDL Temp: 250
Block Temp: 200

Equipment: GK11010007
Interface Bias: +4.5 kV
Drying Gas Flow: 5 L/min
T.Flow: 0.2 ml/min
B.conc: 50% H2O/50% MeOH