

Sample Name :mTRP-2(180-188)
 Cat No. :RP20250
 Lot No. :E3156820E
 Time Processed: 2:01:17 PM
 Month-Day-Year Processed :05/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
32.00	Pumps	Solvent B Conc.	95
32.01	Pumps	Solvent B Conc.	15
42.00	Pumps	Solvent B Conc.	15
95.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ19010325

<Chromatogram>

mV

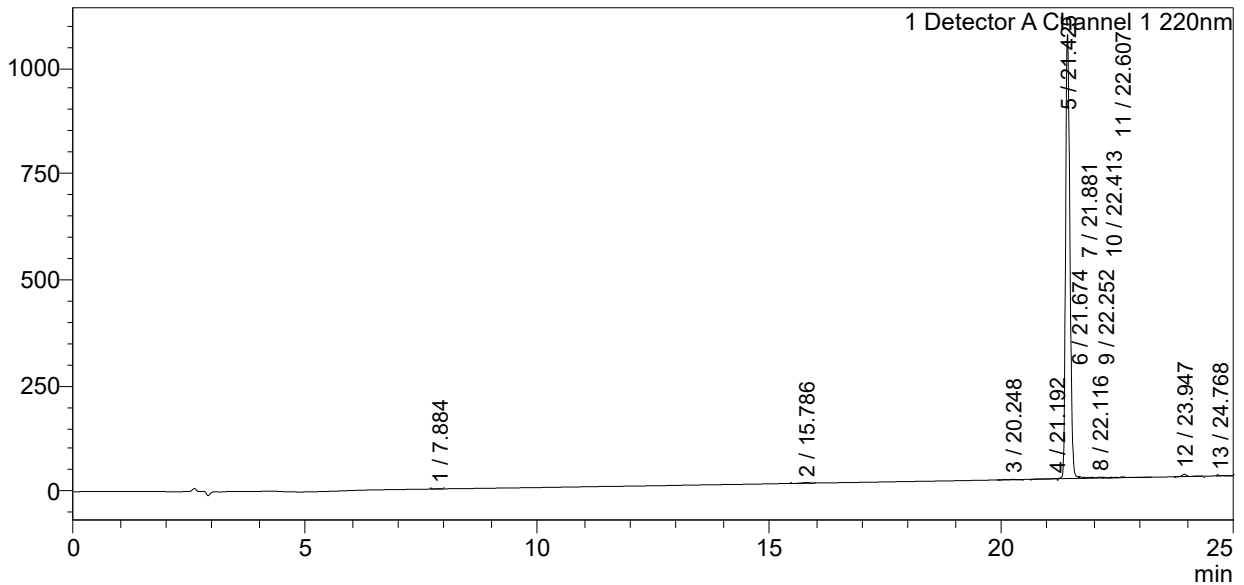

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	7.884	2173	356	0.031
2	15.786	15523	1731	0.222
3	20.248	9708	770	0.139
4	21.192	5854	349	0.084
5	21.425	6813538	1047867	97.632
6	21.674	27479	4452	0.394
7	21.881	14637	2002	0.210
8	22.116	19636	2397	0.281
9	22.252	7969	1347	0.114
10	22.413	5665	933	0.081
11	22.607	16797	1895	0.241
12	23.947	37134	5539	0.532
13	24.768	2705	524	0.039
Total		6978820	1070161	100.000