

Sample Name : Osteogenic Growth Peptide, OGP  
 Cat. No. : RP20311  
 Lot. No. : PE0301811  
 Time Processed : 8:57:27  
 Month-Day-Year Processed : 11/14/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

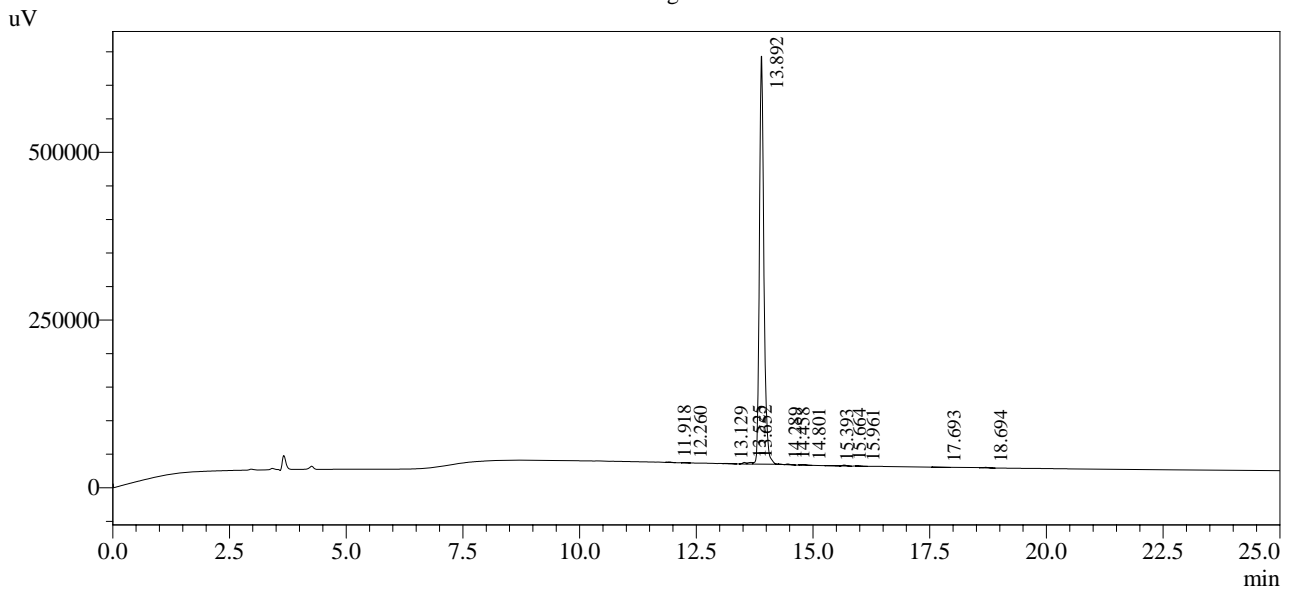

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.918	4103	812	0.099
2	12.260	1271	261	0.031
3	13.129	3410	343	0.082
4	13.525	13009	2298	0.313
5	13.652	15751	2390	0.379
6	13.892	4084894	608087	98.335
7	14.289	906	248	0.022
8	14.458	6186	1076	0.149
9	14.801	4367	654	0.105
10	15.393	1655	263	0.040
11	15.664	7666	1341	0.185
12	15.961	1297	285	0.031
13	17.693	2616	346	0.063
14	18.694	6929	851	0.167
Total		4154061	619256	100.000