

Sample Name :Gastrin-Releasing Peptide, human
 Cat No. :RP10791
 Lot No. :E3875820I
 Time Processed :0:55:57
 Month-Day-Year Processed :09/14/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

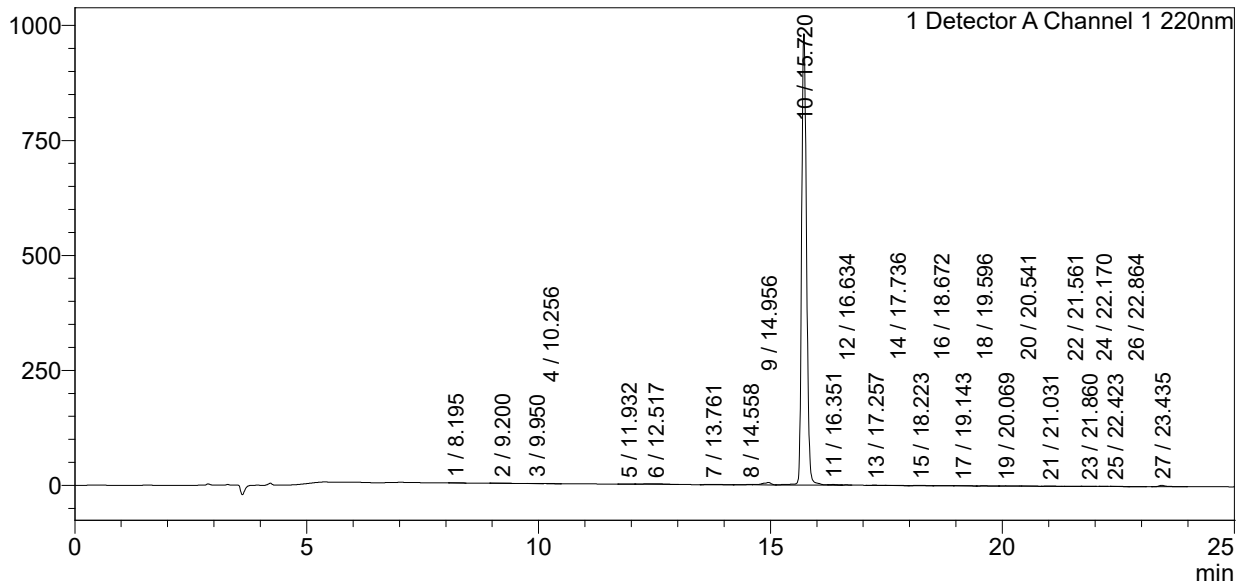

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.195	2431	224	0.033
2	9.200	6215	398	0.083
3	9.950	3836	281	0.052
4	10.256	2325	251	0.031
5	11.932	6345	408	0.085
6	12.517	40170	1314	0.539
7	13.761	19584	809	0.263
8	14.558	11087	820	0.149
9	14.956	71947	5300	0.966
10	15.720	7176412	981667	96.362
11	16.351	5777	862	0.078
12	16.634	2229	375	0.030
13	17.257	4404	349	0.059
14	17.736	7844	574	0.105

Peak#	Ret. Time	Area	Height	Area%
15	18.223	9529	628	0.128
16	18.672	5251	363	0.071
17	19.143	7472	458	0.100
18	19.596	4198	277	0.056
19	20.069	6987	449	0.094
20	20.541	4255	334	0.057
21	21.031	5420	369	0.073
22	21.561	1836	154	0.025
23	21.860	2167	229	0.029
24	22.170	1564	170	0.021
25	22.423	6353	472	0.085
26	22.864	1162	111	0.016
27	23.435	30564	2854	0.410
Total		7447367	1000499	100.000