


Mass Spectrum

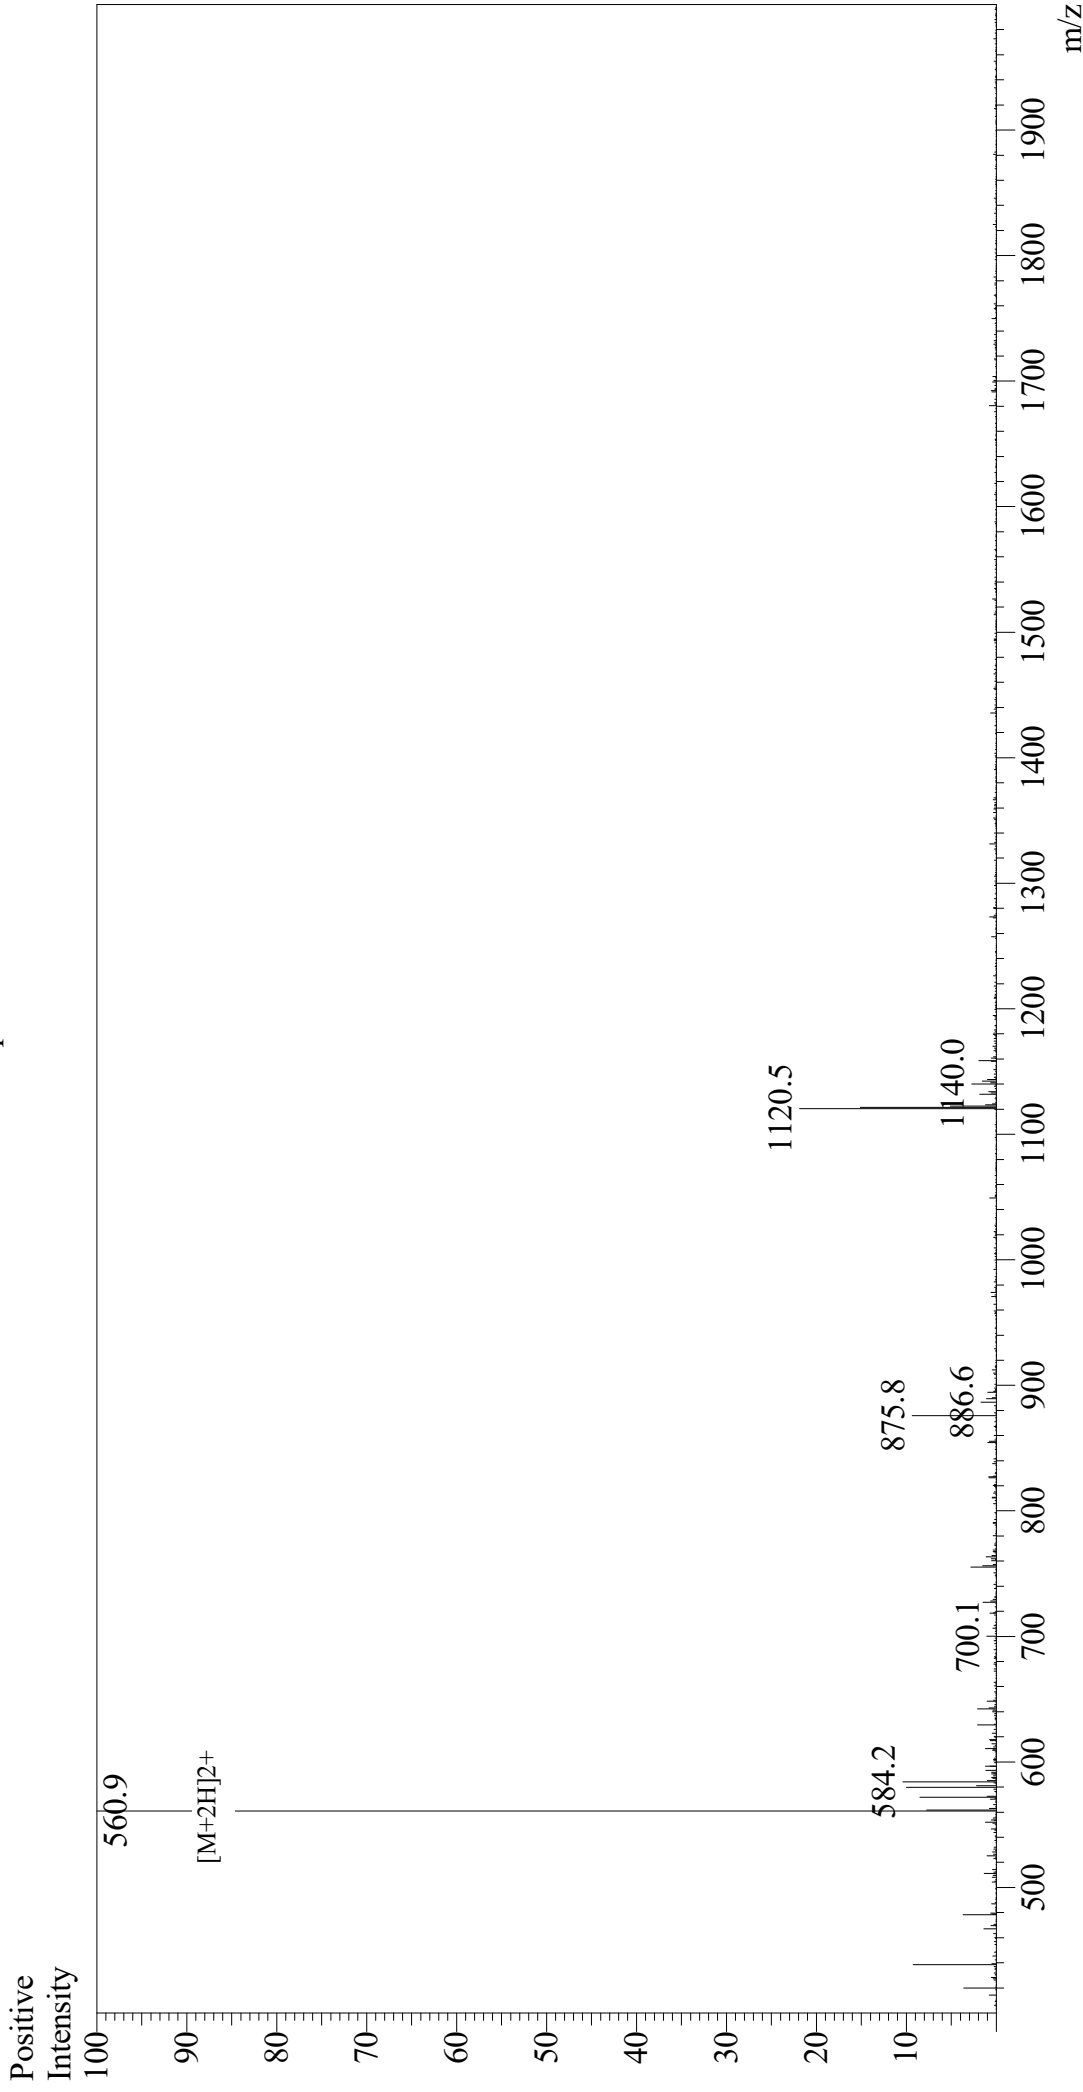

Sample Information	Equipment	: GK11010007
Month-Day Processed :	Interface Bias	: +4.5 kV
Time Processed :	Drying Gas Flow	: 5 L/min
Injection Volume :	T.Flow	: 0.2 ml/min
Sample Name :	B.conc	: 50% H2O/50% MeOH
Cat. No. :	Interface	: ESI
Lot. No. :	Nebulizing Gas Flow	: 1.5 L/min
Theoretical MW :	CDL Temp	: 250
Observed MW :	Block Temp	: 200

01/10/21	Human Papillomavirus (HPV) E7 protein (49 - 57)
1:27:41 PM	
0.3	
RP20249	
E2006921A	
1120.27	
1119.8	