

Sample Name : β -Endorphin, human
 Cat. No. : RP11344
 Lot. No. : PE5671810
 Time Processed :13:58:39
 Month-Day-Year Processed :11/24/2018

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GR11010440

Chromatogram

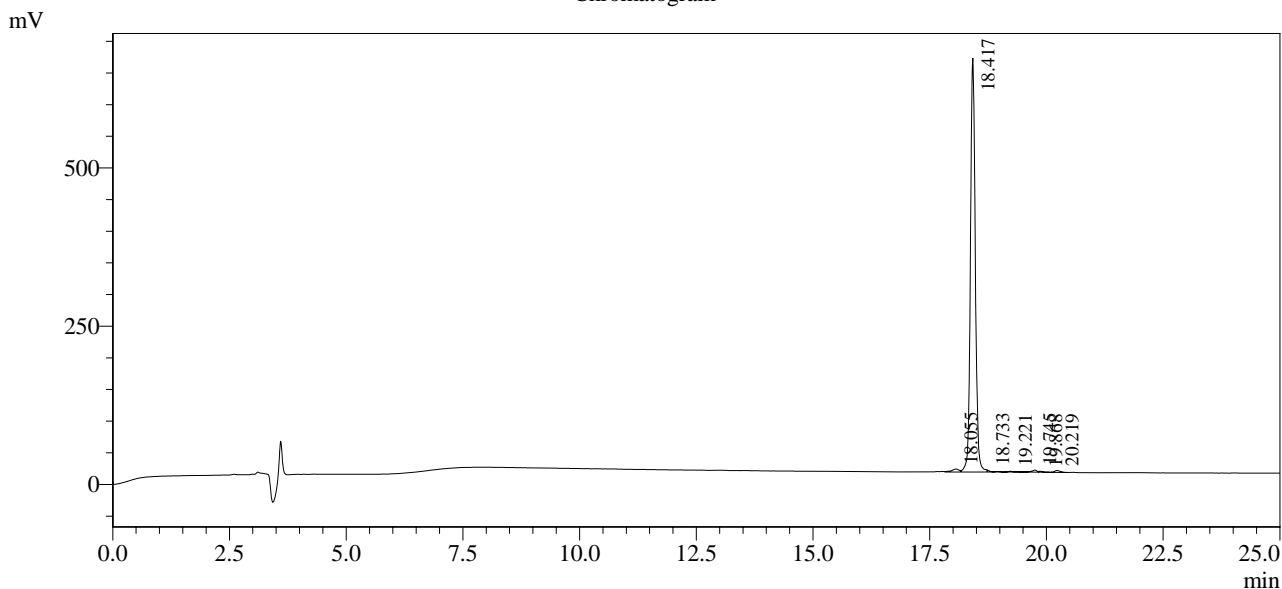

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	18.055	52277	4675	1.067
2	18.417	4766252	653586	97.297
3	18.733	11176	3166	0.228
4	19.221	9359	1219	0.191
5	19.745	26544	3200	0.542
6	19.868	8110	1345	0.166
7	20.219	24944	2874	0.509
Total		4898662	670064	100.000