

Sample Name : Calcitonin Gene Related Peptide (CGRP) (8-37), human
 Cat No. : U0964EF300-1
 Lot No. :
 Time Processed : 6:54:37
 Month-Day-Year Processed : 07/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
25.00	Pumps	Pump B Conc.	65
25.01	Pumps	Pump B Conc.	95
27.00	Pumps	Pump B Conc.	95
27.01	Pumps	Pump B Conc.	5
32.00	Pumps	Pump B Conc.	5
32.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK12010012

<Chromatogram>

mV

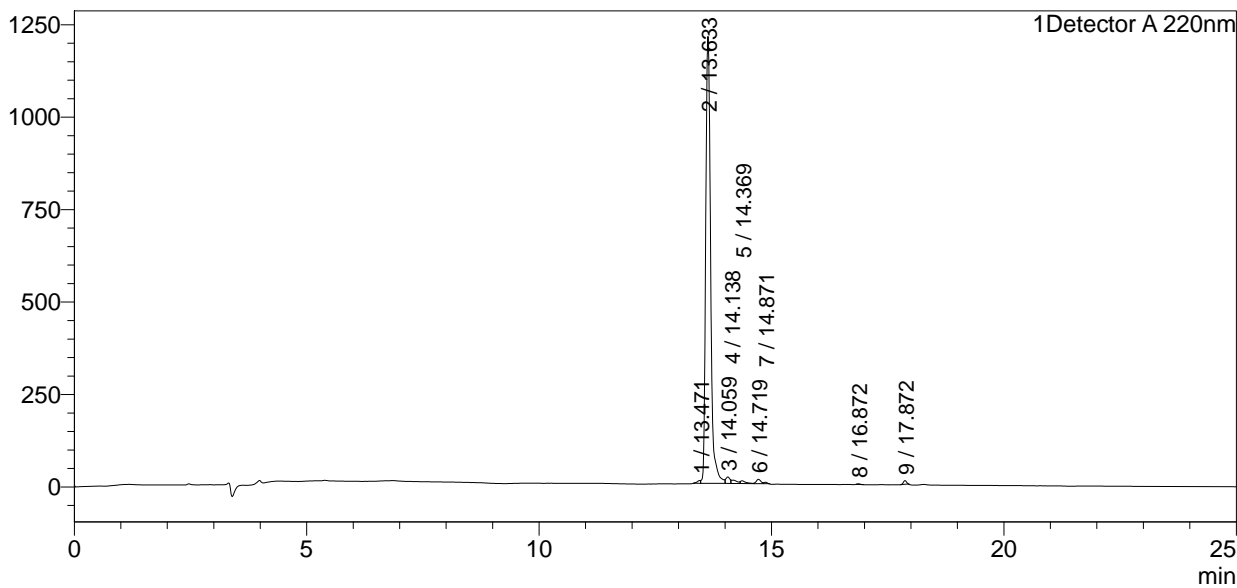

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.471	38010	7522	0.408
2	13.633	8893213	1208339	95.366
3	14.059	105120	17628	1.127
4	14.138	79568	8950	0.853
5	14.369	58763	7528	0.630
6	14.719	77874	11813	0.835
7	14.871	19097	3863	0.205
8	16.872	6261	1536	0.067
9	17.872	47453	9877	0.509
Total		9325360	1277055	100.000