

Sample Name :Kisspeptin-10
 Cat No :RP20494
 Lot No :E6306920L
 Time Processed :2:52:34
 Month-Day-Year Processed :12/23/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: SS-CM-0309

<Chromatogram>

mV

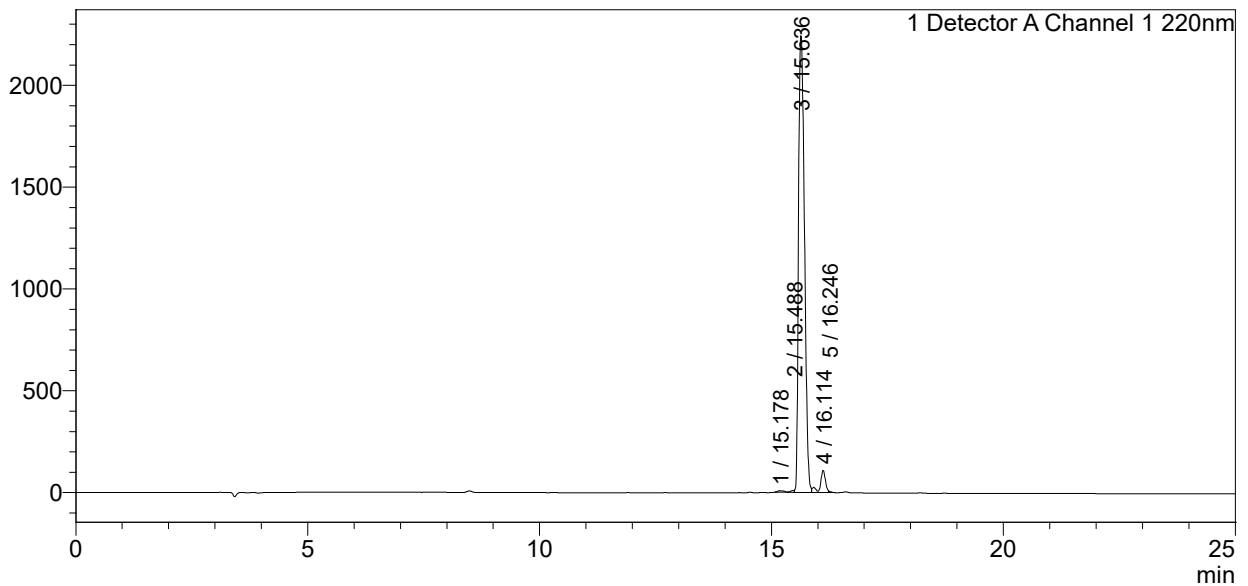

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.178	74052	7436	0.354
2	15.488	48443	9044	0.232
3	15.636	19912543	2243556	95.224
4	16.114	854711	109015	4.087
5	16.246	21444	6546	0.103
Total		20911193	2375596	100.000