

Sample Name :Glucagon (19-29), human
 Cat No. :RP10770
 Lot No. :E1394421G
 Time Processed :21:04:03
 Month-Day-Year Processed :07/21/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm
 <<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

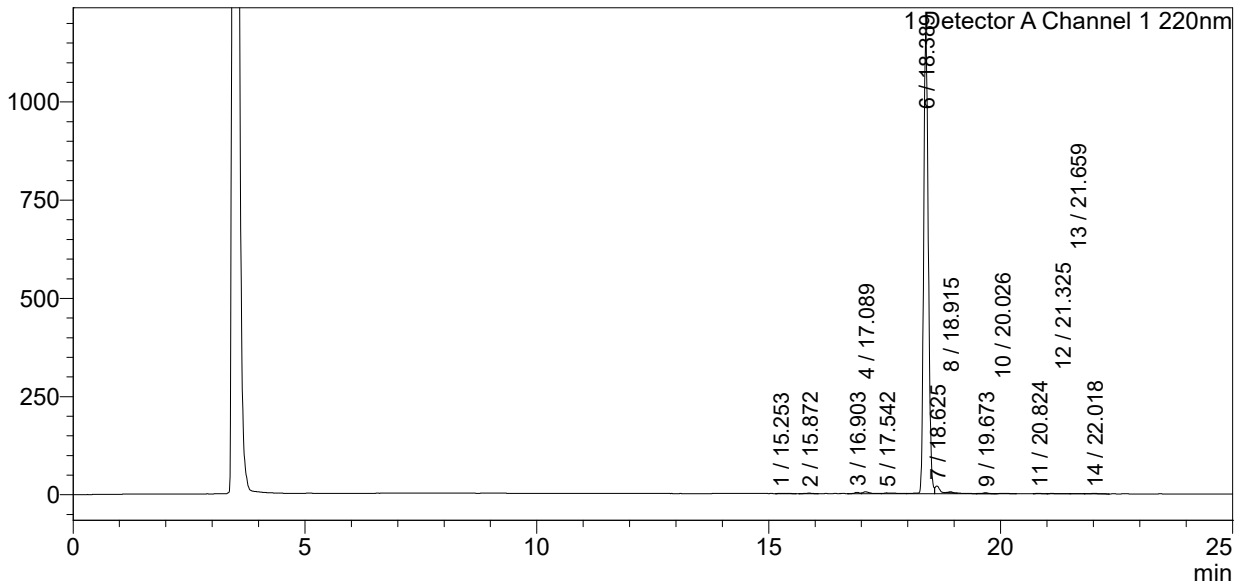

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	15.253	5301	358	0.062
2	15.872	9943	1189	0.116
3	16.903	22635	3108	0.263
4	17.089	44417	4579	0.516
5	17.542	28727	1809	0.334
6	18.389	8226222	1158950	95.625
7	18.625	190761	18935	2.217
8	18.915	16188	2701	0.188
9	19.673	17732	2120	0.206
10	20.026	8789	763	0.102
11	20.824	4397	583	0.051
12	21.325	8288	338	0.096
13	21.659	6301	596	0.073
14	22.018	12893	1348	0.150

Peak#	Ret. Time	Area	Height	Area%
Total		8602593	1197377	100.000