


Mass Spectrum

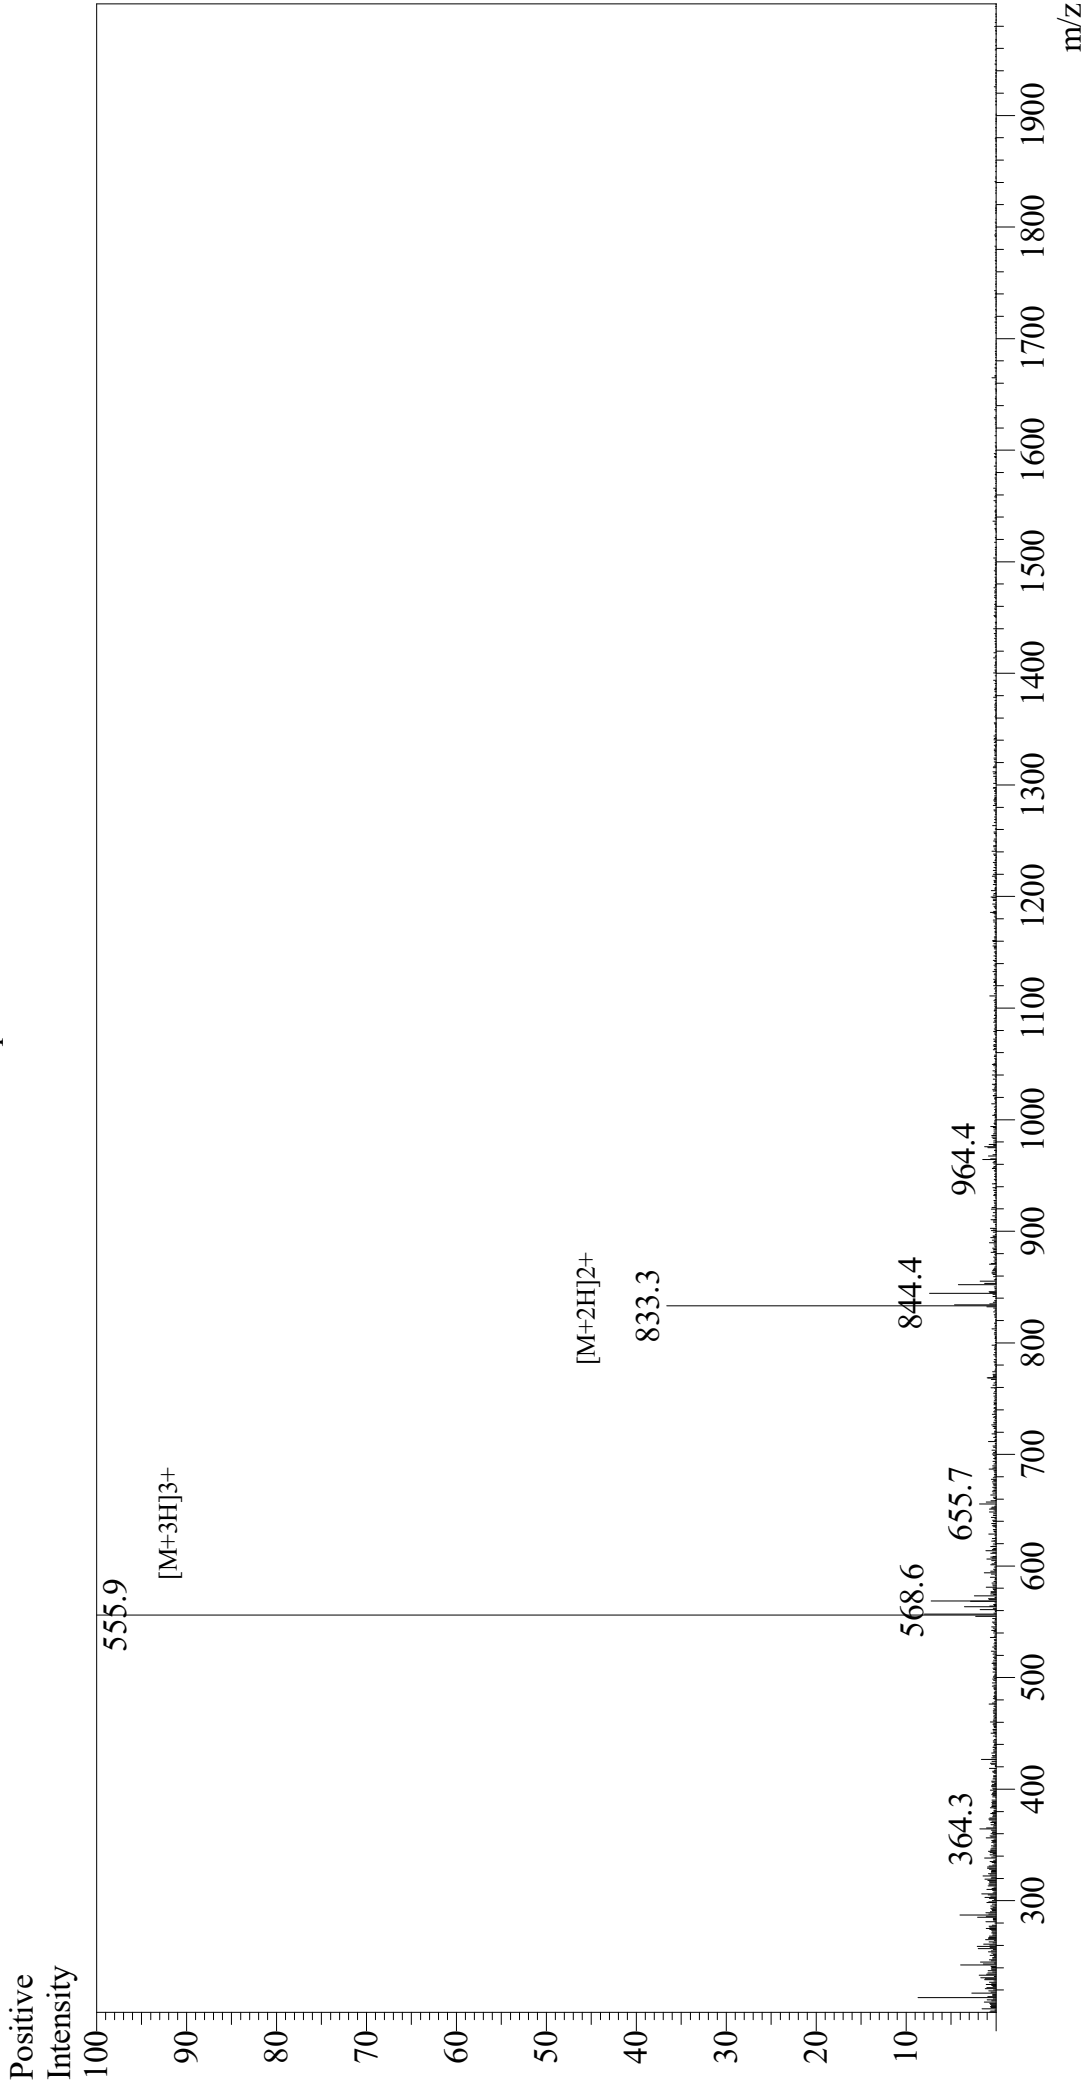

Sample Information

Acquired by : Gary
 Month-Day Processed : 01/09/19
 Time Processed : 04:44:18 PM
 Injection Volume : 0.2
 Sample Name : α -Melanocyte-Stimulating Hormone (MSH), amide
 Cat No. : RP10644
 Lot No. : PE9361901
 Theoretical MW : 1664.90
 Observed MW : 1664.7

Interface : ESI
 Nebulizing Gas Flow : 1.5L/min
 CDL Temp : 250
 Block Temp : 200
 Equipment : GK11010007
 Interface Bias : +4.5 kV
 Drying Gas Flow : 5 L/min
 T.Flow : 0.2 ml/min
 B.conc : 50% H₂O/50% MeOH