

Sample Name :Angiotensin II (1-4), human
 Cat No. :RP11252
 Lot No. :E6150220J
 Time Processed :22:52:37
 Month-Day-Year Processed :10/20/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

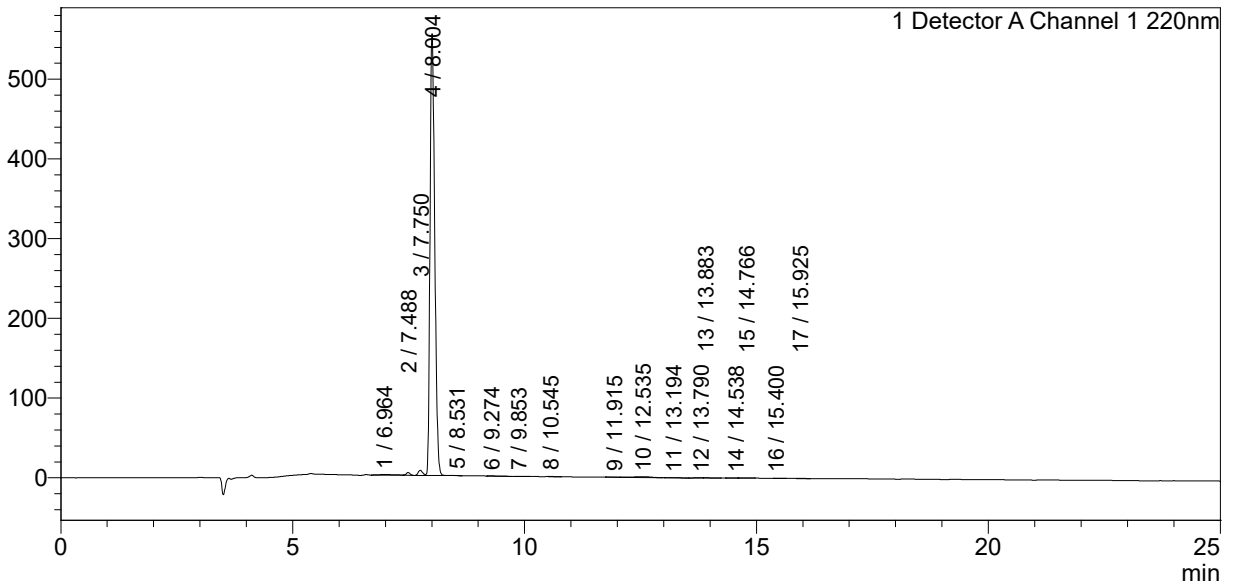

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	6.964	15489	648	0.379
2	7.488	18678	3305	0.457
3	7.750	42647	6419	1.044
4	8.004	3939502	554378	96.423
5	8.531	1756	351	0.043
6	9.274	3630	152	0.089
7	9.853	1365	130	0.033
8	10.545	1041	124	0.025
9	11.915	4466	304	0.109
10	12.535	33758	1120	0.826
11	13.194	5674	375	0.139
12	13.790	5805	456	0.142
13	13.883	4514	430	0.110
14	14.538	1492	152	0.037

Peak#	Ret. Time	Area	Height	Area%
15	14.766	2562	199	0.063
16	15.400	1359	119	0.033
17	15.925	1913	187	0.047
Total		4085651	568848	100.000