

Sample Name :Osteogenic Growth Peptide, OGP
 Cat No. :RP20311
 Lot No. :E7160720G
 Time Processed :9:18:25
 Month-Day-Year Processed :07/09/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>
 Column : Alltima™ C18 4.6 x 250 mm
 Equipment:ZJ19010141

<Chromatogram>

mV

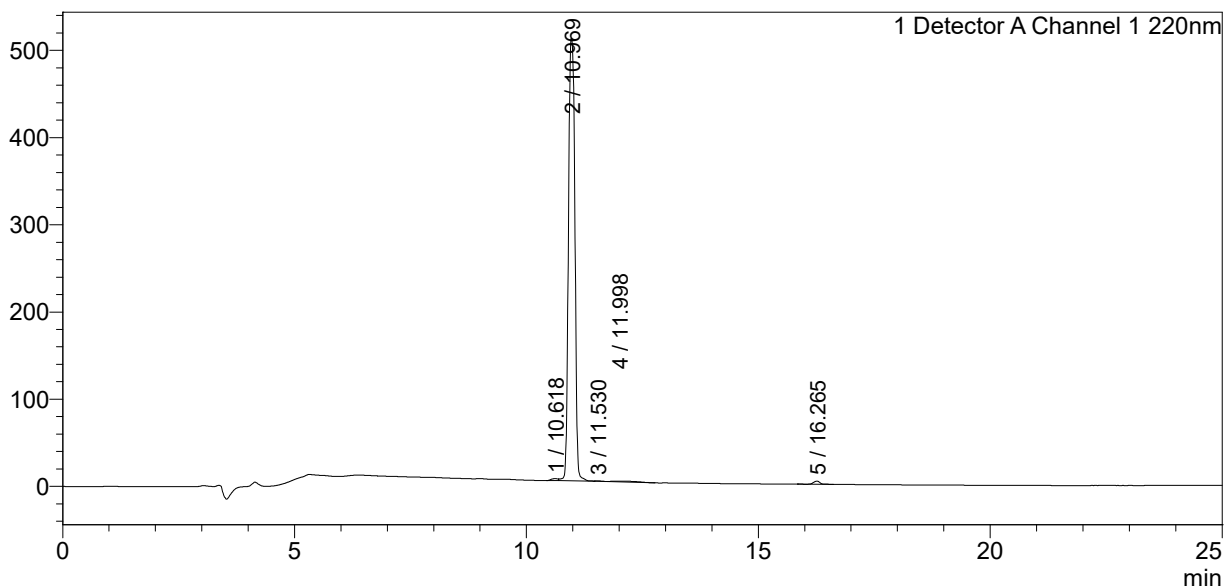

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.618	23211	2383	0.472
2	10.969	4829743	507685	98.152
3	11.530	2010	231	0.041
4	11.998	32556	804	0.662
5	16.265	33172	3625	0.674
Total		4920693	514728	100.000