


Mass Spectrum

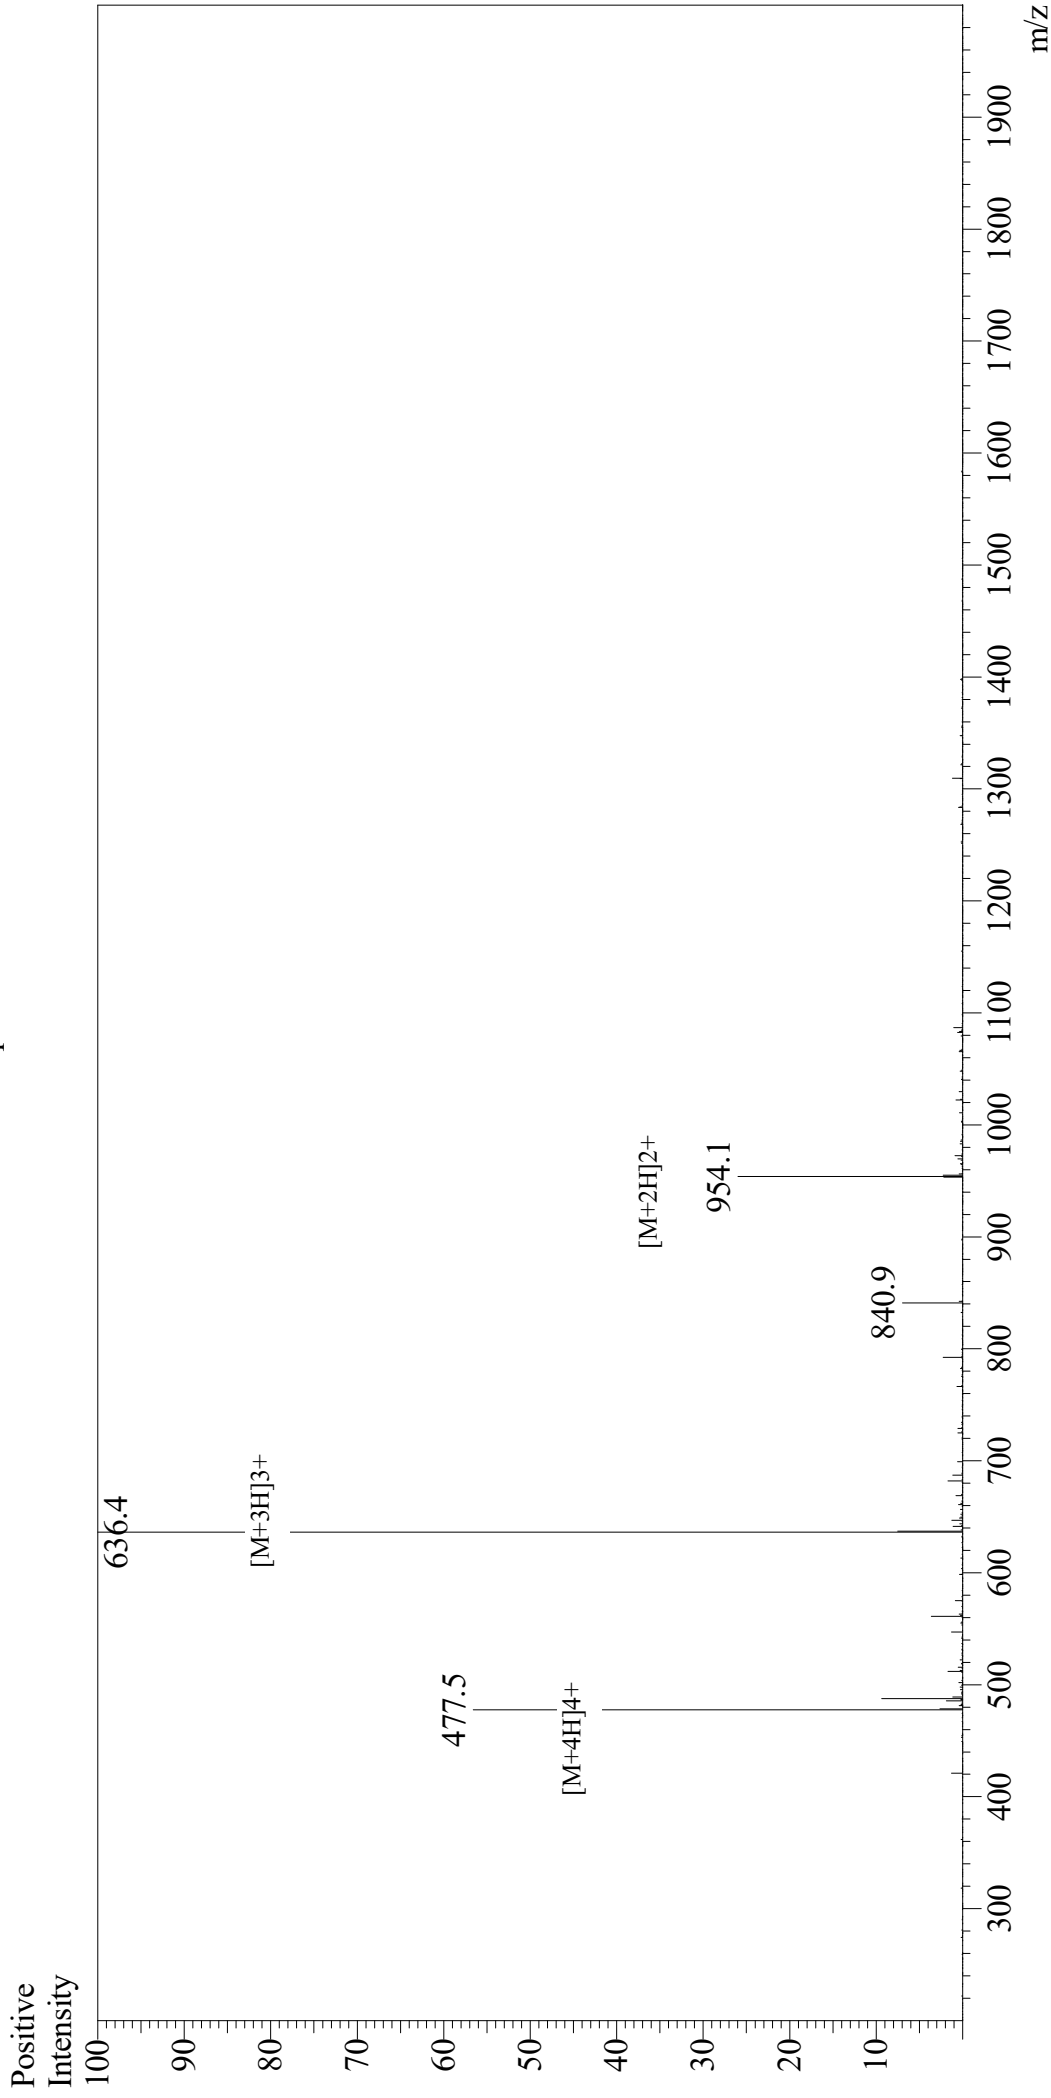

Sample Information

User : Gary
Month-Day Processed : 03/02/19
Time Processed : 01:15:35 PM
Injection Volume : 0.2
Sample Name : Indolicidin
Cat No. : RP11242
Lot No. : PE8431902
Theoretical MW : 1906.28
Observed MW : 1906.2

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH