

Sample Name :HIV p17 Gag (77-85)  
 Cat. No. : RP17316  
 Lot. No. :E7025519J  
 Time Processed :9:08:59  
 Month-Day-Year Processed :10/03/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment :SS-CM-0310

Chromatogram

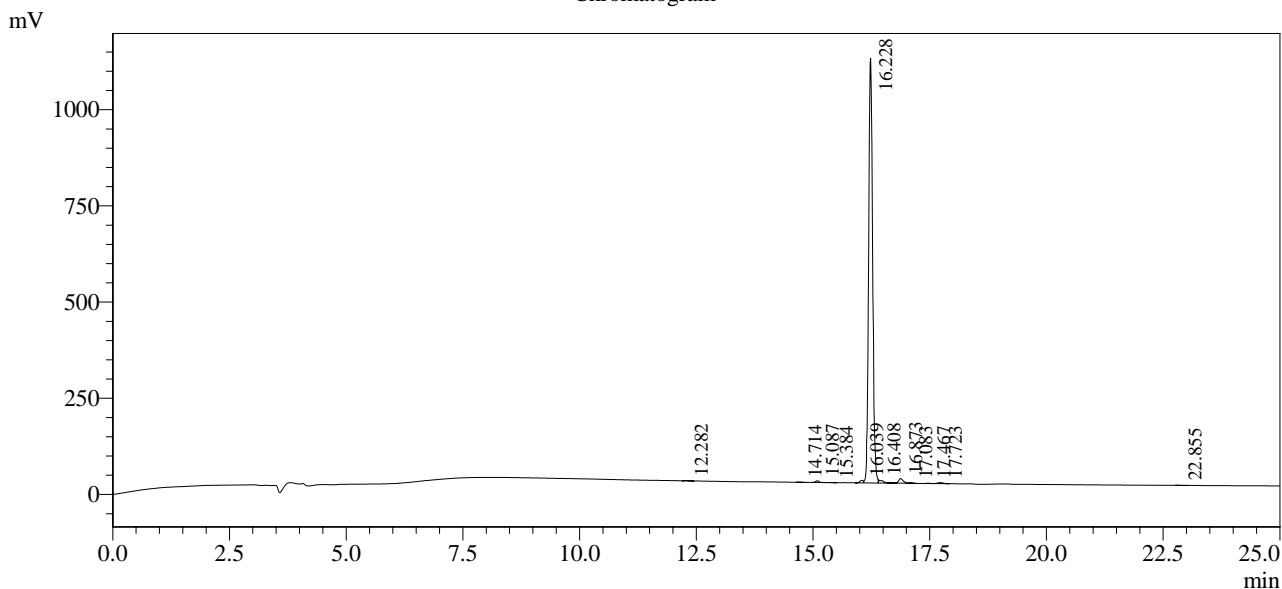

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	12.282	3924	718	0.058
2	14.714	3043	576	0.045
3	15.087	24157	4570	0.359
4	15.384	1008	232	0.015
5	16.039	33187	6569	0.493
6	16.228	6504869	1103774	96.605
7	16.408	50409	7431	0.749
8	16.873	84194	12081	1.250
9	17.083	1129	295	0.017
10	17.467	3990	778	0.059
11	17.723	21431	2725	0.318
12	22.855	2164	329	0.032
Total		6733504	1140077	100.000