

Sample Name: Uty HY Peptide (246-254)  
 Cat No. : RP20261  
 Lot No. : E4564219K  
 Time Processed : 19:51:27  
 Month-Day-Year Processed : 11/17/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow: 1 ml/min  
 Wavelength: 220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ17010508

<Chromatogram>

mV

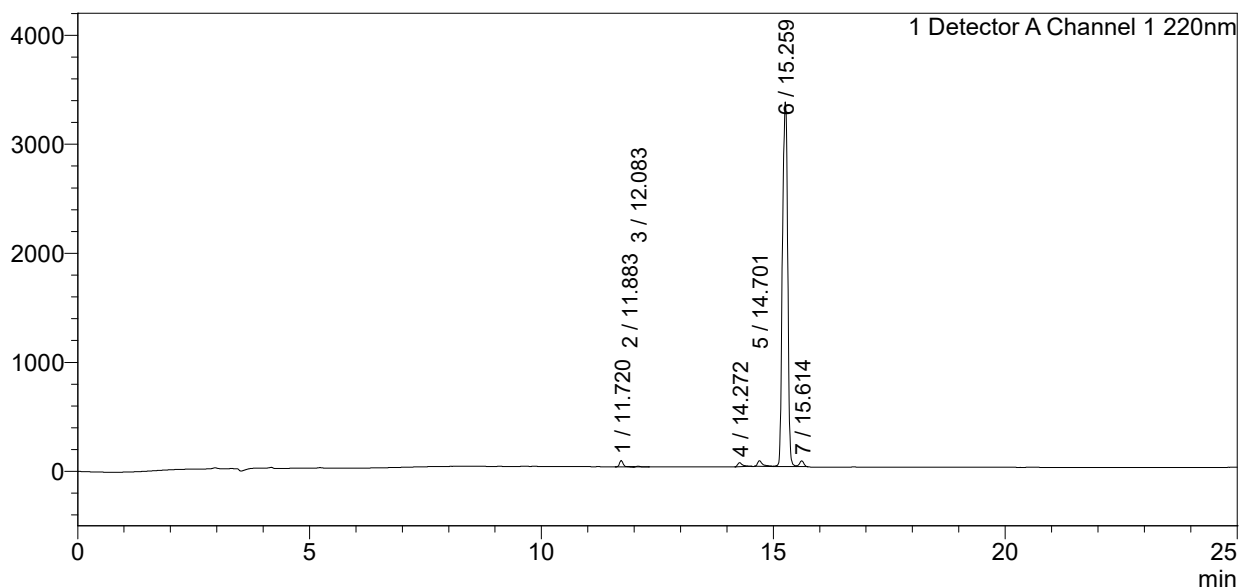

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.720	305374	57036	1.111
2	11.883	1513	476	0.006
3	12.083	30230	5926	0.110
4	14.272	273729	37043	0.996
5	14.701	411545	52300	1.498
6	15.259	26104432	3342487	95.013
7	15.614	347891	53478	1.266
Total		27474714	3548746	100.000