


# Mass Spectrum

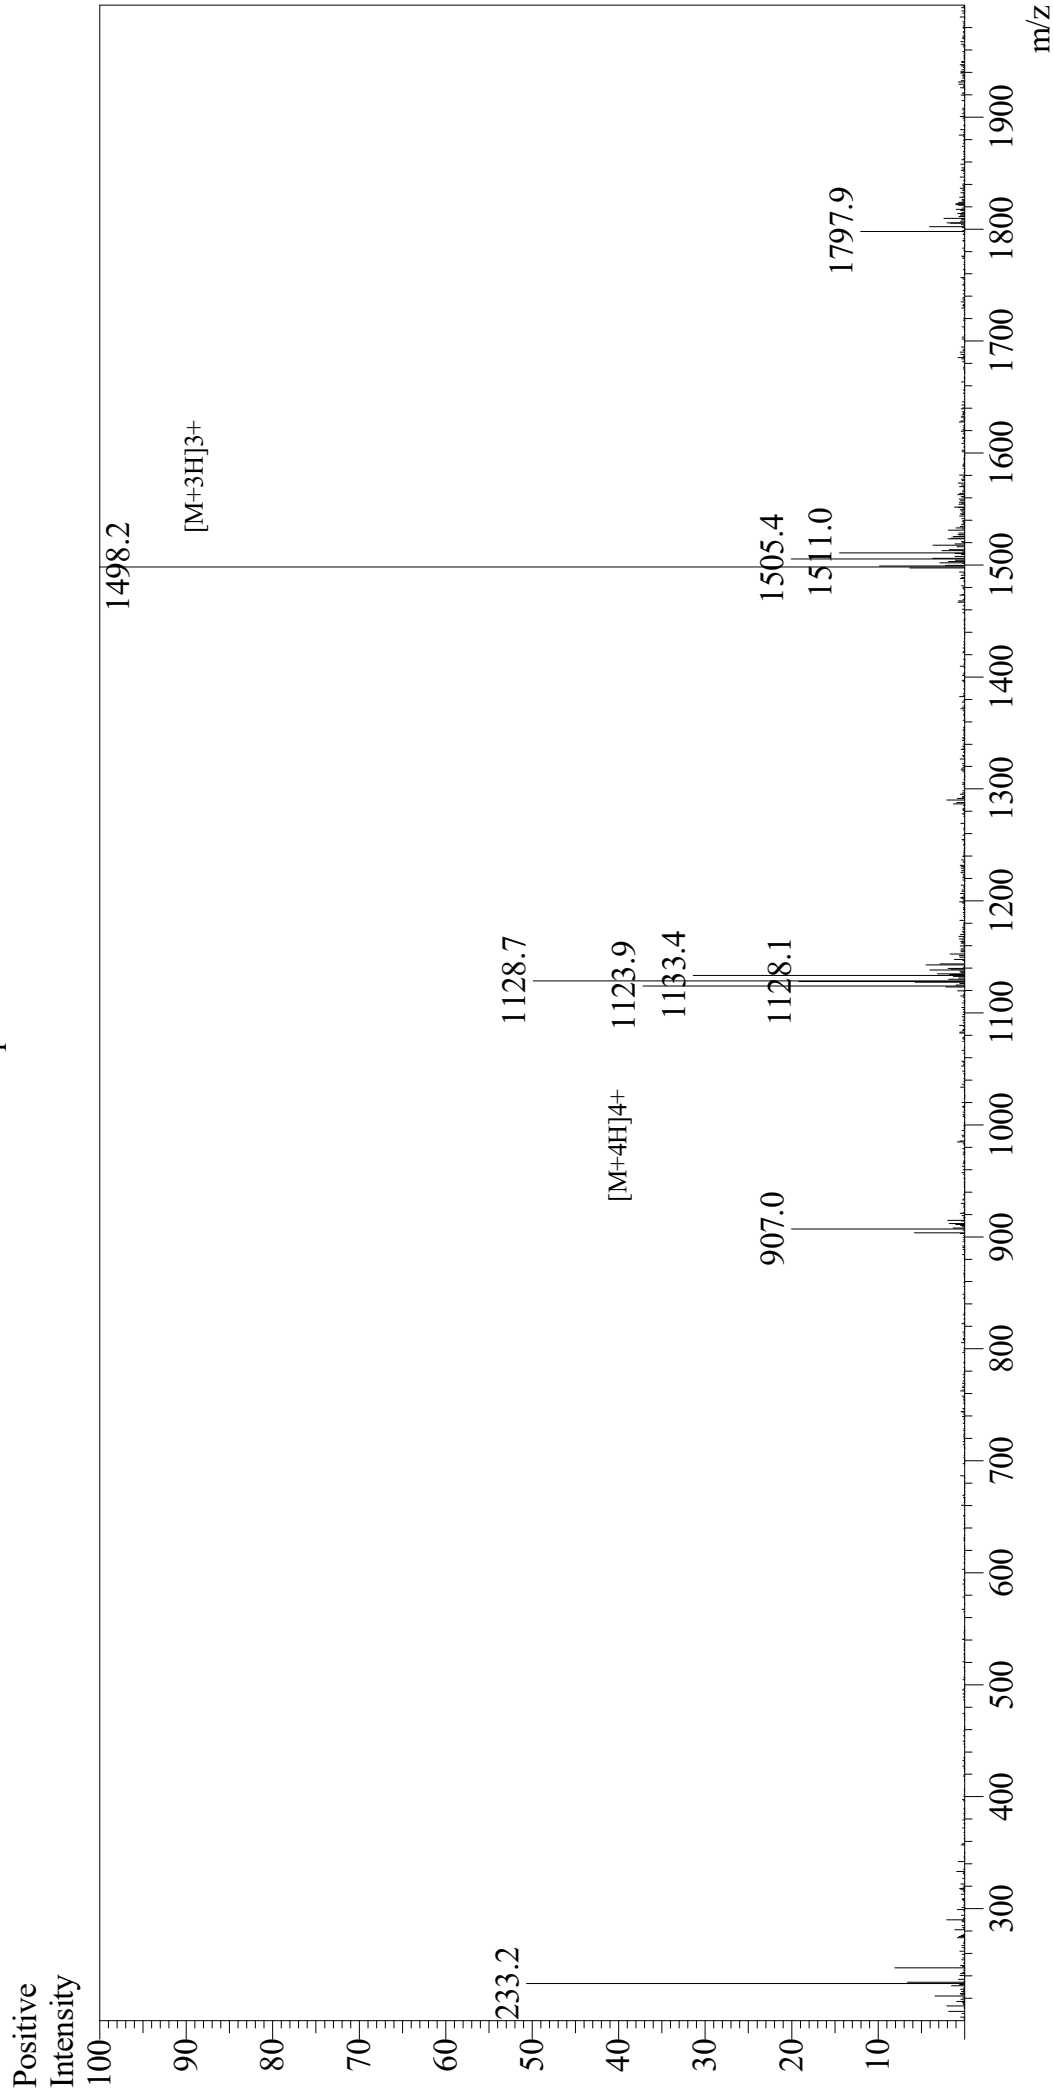

## Sample Information

User : Gary  
 Month-Day Processed : 01/26/19  
 Time Processed : 03:47:59 PM  
 Injection Volume : 0.3  
 Sample Name : Enfuvirtide (T-20)  
 Cat No. : RP17307  
 Lot No. : PE4281901  
 Theoretical MW : 4491.88  
 Observed MW : 4491.6

Interface : ESI  
 Nebulizing Gas Flow : 1.5L/min  
 CDL Temp : 250  
 Block Temp : 200

Equipment : GK11010007  
 Interface Bias : +4.5kV  
 Drying Gas Flow : 5 L/min  
 T.Flow : 0.2ml/min  
 B.conc : 50%H2O/50%MeOH