

Sample Name :PTD-p65-P1 Peptide  
 Cat No. :RP20522  
 Lot No. :E4942719I  
 Time Processed :8:21:10 AM  
 Month-Day-Year Processed :09/26/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
35.00	Pumps	Solvent B Conc.	5
35.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

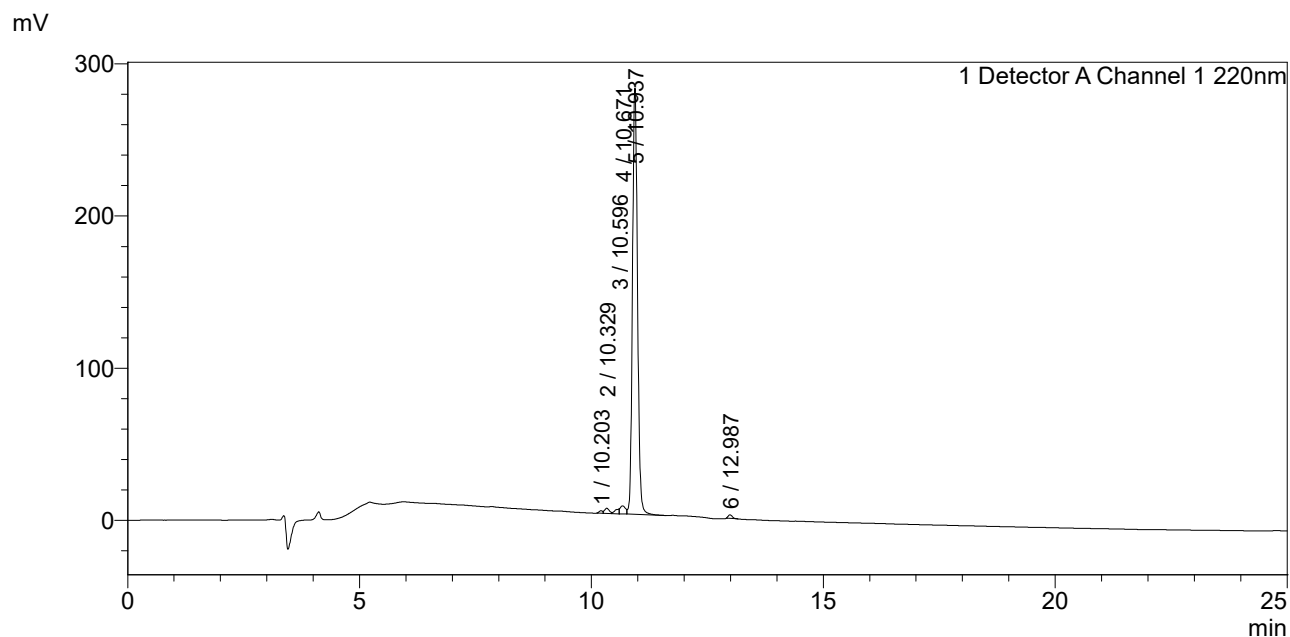

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.203	8241	1587	0.372
2	10.329	23960	3402	1.081
3	10.596	20312	3058	0.917
4	10.671	42536	5315	1.920
5	10.937	2106169	280304	95.055
6	12.987	14510	2434	0.655
Total		2215728	296100	100.000