

Sample Name : Melittin  
 Cat. No. : RP10290  
 Lot. No. : E5867320C  
 Time Processed :22:23:20  
 Month-Day-Year Processed :03/28/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010009

Chromatogram

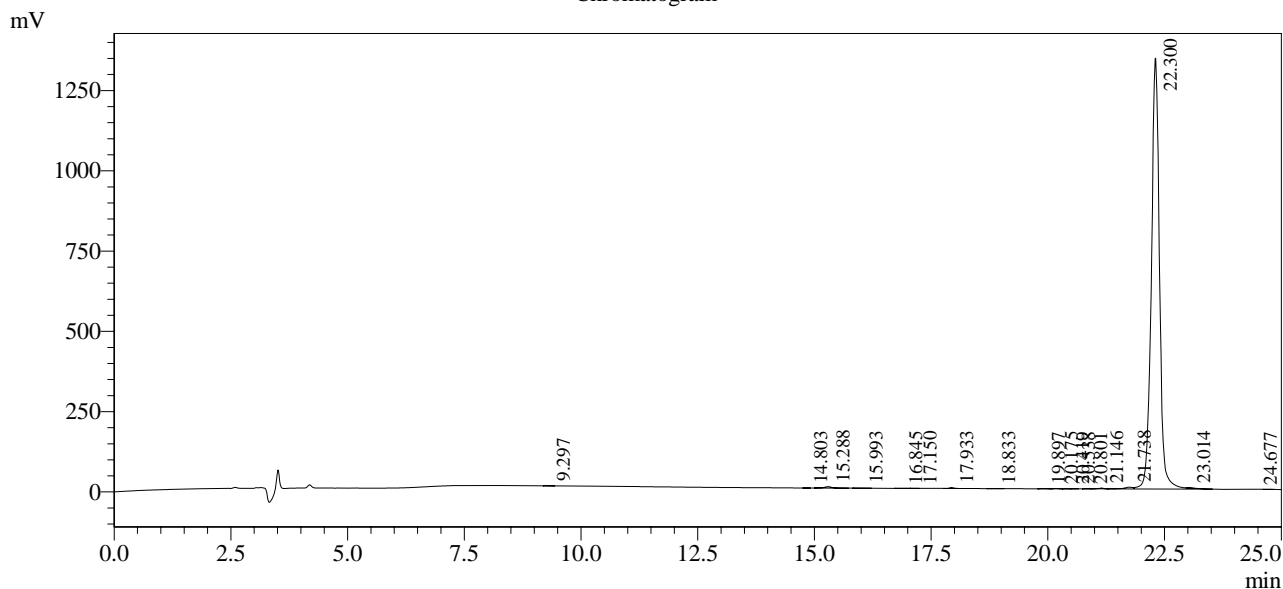

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.297	1823	283	0.011
2	14.803	1104	141	0.007
3	15.288	50090	4370	0.303
4	15.993	5971	540	0.036
5	16.845	1159	117	0.007
6	17.150	1401	195	0.008
7	17.933	20840	2898	0.126
8	18.833	1950	146	0.012
9	19.897	1669	195	0.010
10	20.175	6017	1069	0.036
11	20.419	1058	139	0.006
12	20.538	1048	184	0.006
13	20.801	1129	197	0.007
14	21.146	18488	2545	0.112
15	21.738	70960	5370	0.430
16	22.300	16330382	1341520	98.844
17	23.014	5062	936	0.031
18	24.677	1151	162	0.007
Total		16521300	1361008	100.000