

Sample Name :AMARA peptide  
 Cat No. : RP20472  
 Lot No. :E3669120G  
 Time Processed : 9:50:47  
 Month-Day-Year Processed : 07/19/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
31.00	Pumps	Pump A B.Conc	95
31.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
40.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment:GK12010012

<Chromatogram>

mV

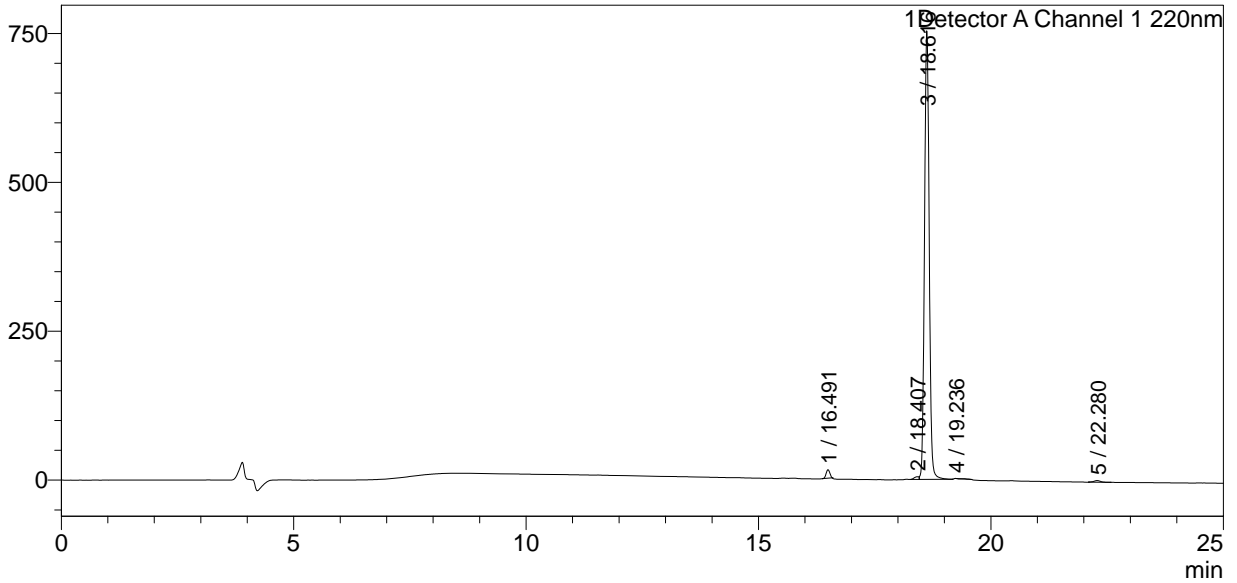

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.491	78574	14214	1.444
2	18.407	31736	4387	0.583
3	18.616	5304754	753117	97.458
4	19.236	2561	149	0.047
5	22.280	25484	2684	0.468
Total		5443109	774550	100.000