

Sample Name :c-Myc Peptide  
 Cat No. :RP11731  
 Lot No. :E2518720J  
 Time Processed :11:38:05  
 Month-Day-Year Processed :10/18/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

<Chromatogram>

mV

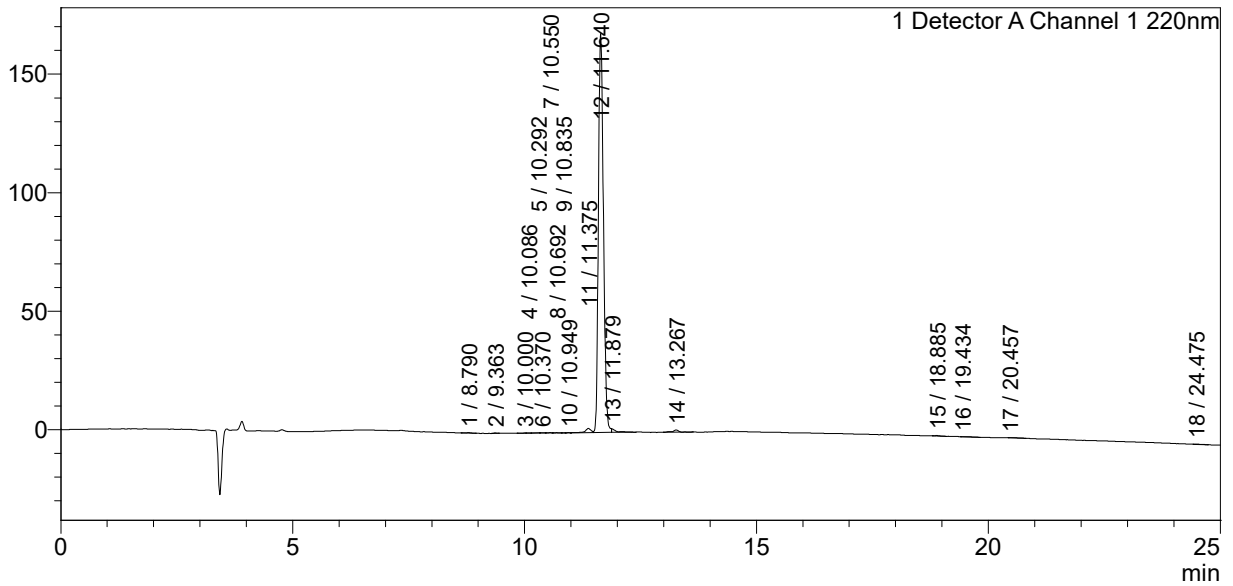

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	8.790	1367	177	0.104
2	9.363	901	159	0.069
3	10.000	366	52	0.028
4	10.086	440	100	0.034
5	10.292	763	96	0.058
6	10.370	587	109	0.045
7	10.550	691	113	0.053
8	10.692	652	75	0.050
9	10.835	143	36	0.011
10	10.949	220	60	0.017
11	11.375	14910	1731	1.140
12	11.640	1264375	168322	96.634
13	11.879	9936	1520	0.759
14	13.267	7325	940	0.560

Peak#	Ret. Time	Area	Height	Area%
15	18.885	1490	191	0.114
16	19.434	1081	42	0.083
17	20.457	1831	113	0.140
18	24.475	1340	130	0.102
Total		1308419	173967	100.000