

Sample Name :Angiotensin II (1-4), human  
 Cat No. :RP11252  
 Lot No. :E2247620J  
 Time Processed :21:20:06  
 Month-Day-Year Processed :10/11/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm  
 Equipment: ZJ19010141

### <Chromatogram>

mV

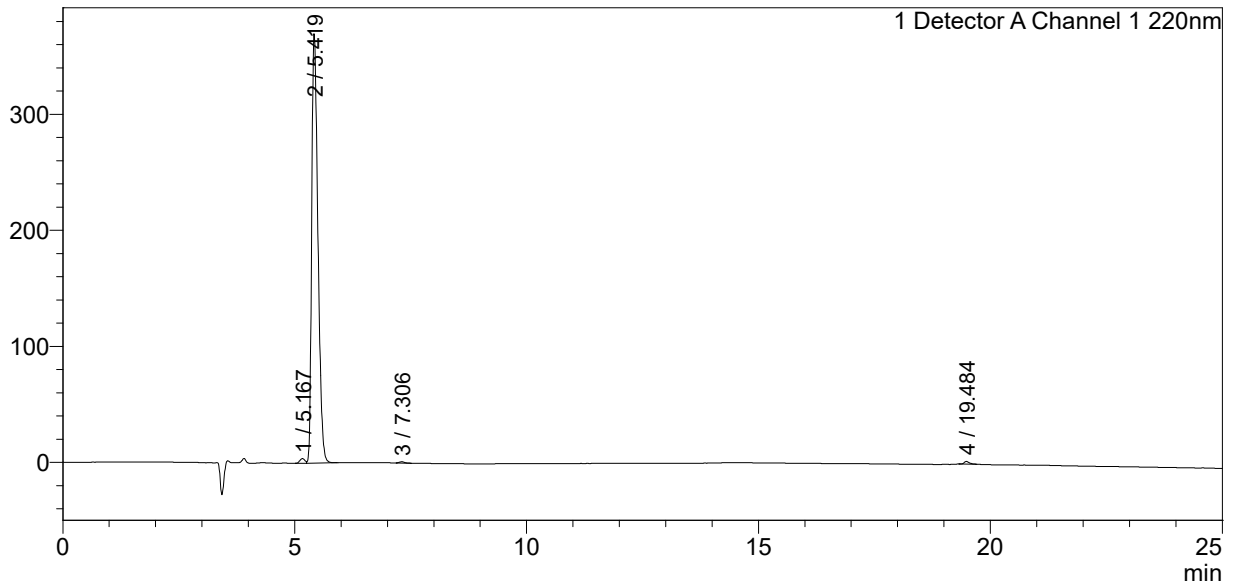

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.167	31678	4091	0.907
2	5.419	3436085	370182	98.399
3	7.306	8084	1072	0.232
4	19.484	16159	2161	0.463
Total		3492008	377506	100.000