


Mass Spectrum

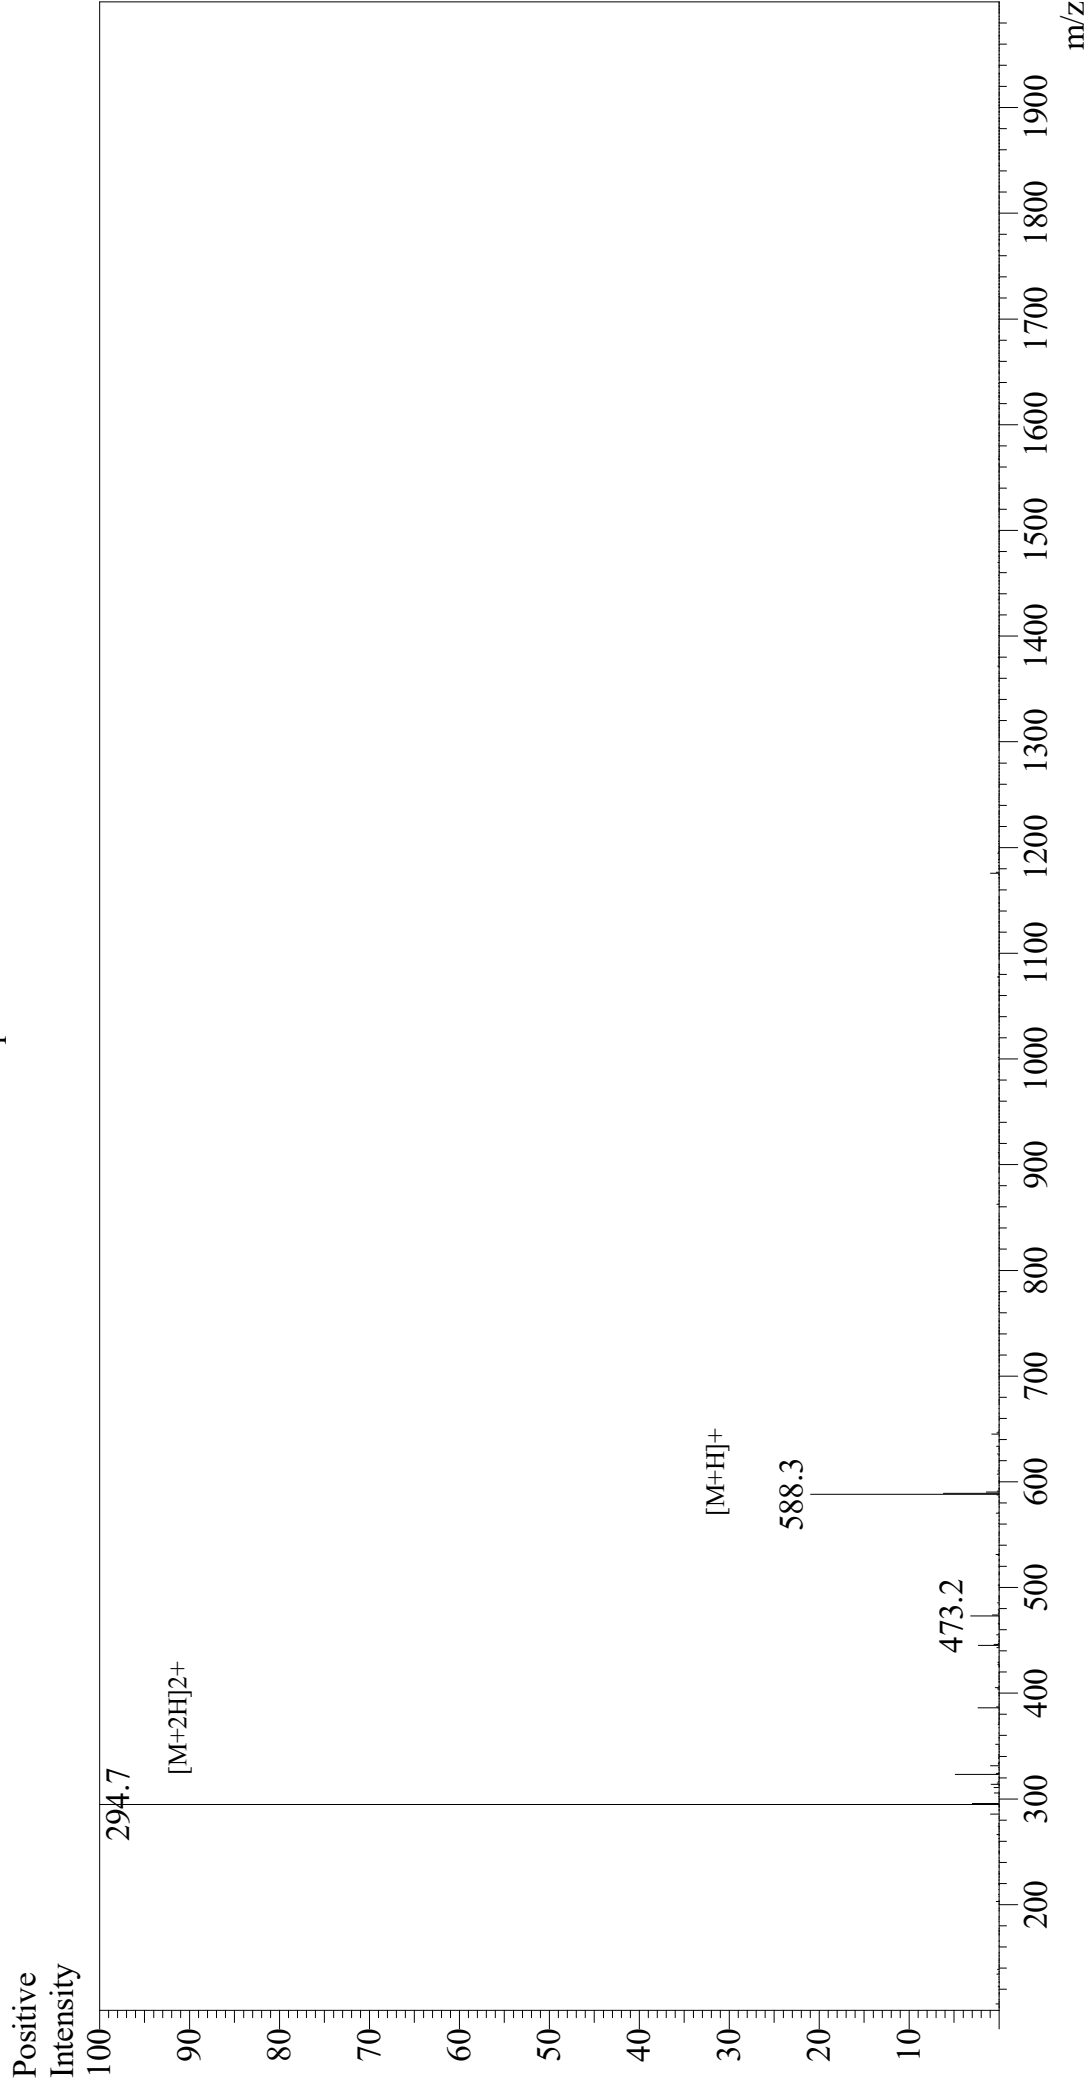

Sample Information

Acquired by : Gary
Month-Day Processed : 04/03/20
Time Processed : 10:22:37 AM
Injection Volume : 0.3
Sample Name : GRGDSF
Cat. No. : RP20255
Lot. No. : E6047520C
Theoretical MW : 587.59
Observed MW : 587.4

Interface : ESI
Nebulizing Gas Flow : 1.5L/min
CDL Temp : 250
Block Temp : 200

Equipment : GK11010007
Interface Bias : +4.5 kV
Drying Gas Flow : 5 L/min
T.Flow : 0.2 ml/min
B.conc : 50% H₂O / 50% MeOH