


Mass Spectrum

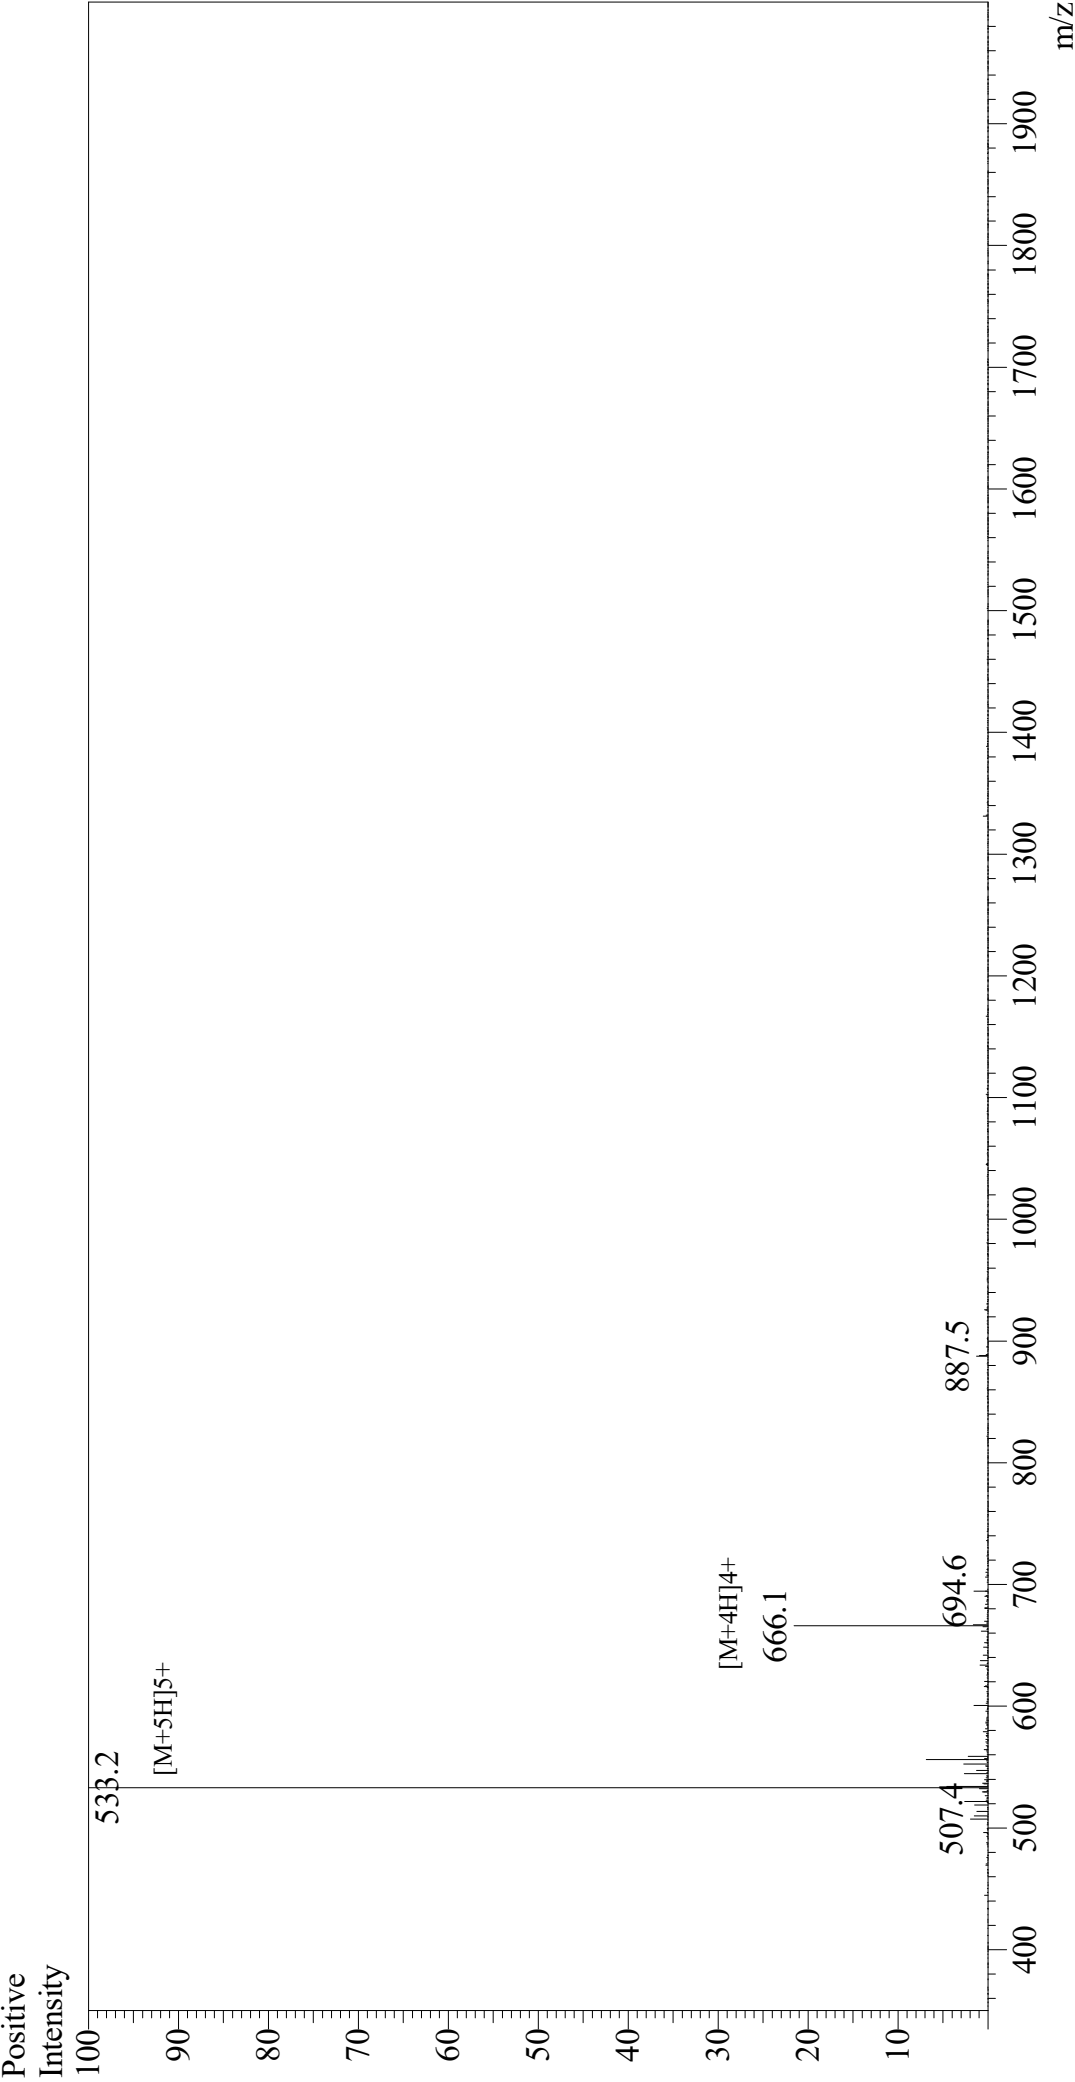

Sample Information		Equipment	
Month-Day Processed :	08/18/21	Interface	: ZJ21010035
Time Processed :	8:49:49	Nebulizing Gas Flow	: +4.5 kV
Injection Volume :	0.2	CDL Temp	: 5 L/min
Sample Name :	$\beta$ -Melanocyte Stimulating Hormone (MSH), human	Drying Gas Flow	: 0.2 ml/min
Cat No. :	RP10648	Block Temp	: 50% H <sub>2</sub> O/50% MeOH
Lot No. :	E8572021H		
Theoretical MW :	2661.00		
Observed MW :	2661.0		