

Sample Name : [Sar1, Ile8]-Angiotensin II
 Cat. No. : RP13720
 Lot. No. : E4909919I
 Time Processed : 10:58:53
 Month-Day-Year Processed : 09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010011

Chromatogram

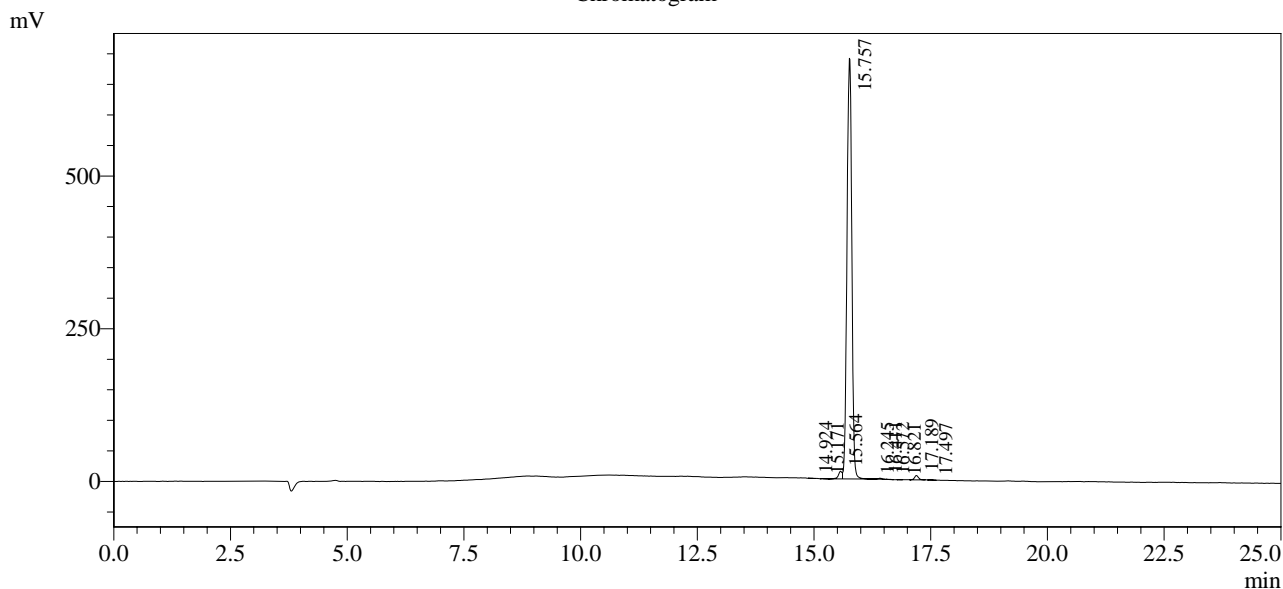

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.924	1064	216	0.021
2	15.171	1107	246	0.022
3	15.564	71077	12600	1.392
4	15.757	4972958	688790	97.427
5	16.245	3492	606	0.068
6	16.411	7953	1446	0.156
7	16.572	1297	186	0.025
8	16.821	1032	216	0.020
9	17.189	42357	7092	0.830
10	17.497	1975	419	0.039
Total		5104313	711816	100.000