

Sample Name : CEF1, Influenza Matrix Protein M1 (58 - 66)
 Cat. No. : RP19978
 Lot. No. : PE8631902
 Time Processed : 4:25:16
 Month-Day-Year Processed : 03/02/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: GK11010017

Chromatogram

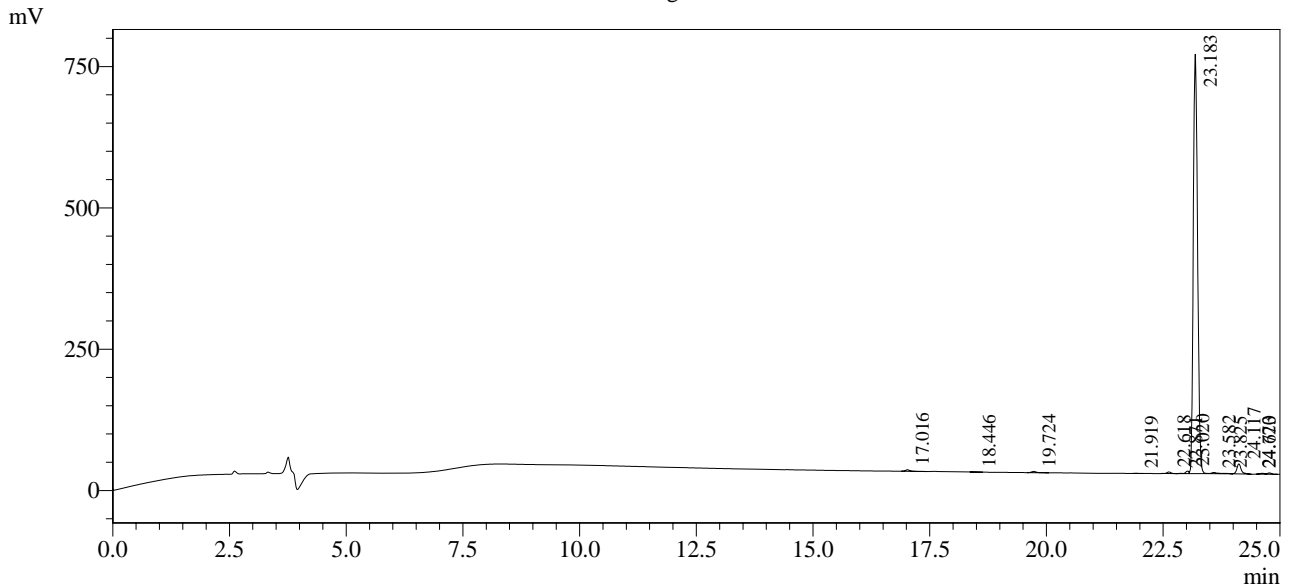

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	17.016	18223	2731	0.365
2	18.446	2554	409	0.051
3	19.724	15273	2129	0.306
4	21.919	1551	293	0.031
5	22.618	16711	2835	0.335
6	22.871	2914	600	0.058
7	23.020	21607	4443	0.433
8	23.183	4755998	741948	95.248
9	23.582	19092	2167	0.382
10	23.825	5152	769	0.103
11	24.117	111029	17530	2.224
12	24.620	9774	1456	0.196
13	24.773	13378	2334	0.268
Total		4993255	779643	100.000