

Sample Name : Exendin (9-39)
 Cat No. : RP10872
 Lot No. : PE4941802

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow: 1 ml/min
 Wavelength: 220 nm

<<LC Time Program>>


Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
41.00	Pumps	Pump B Conc.	95
41.01	Pumps	Pump B Conc.	5
50.00	Pumps	Pump B Conc.	5
50.01	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

<Chromatogram>

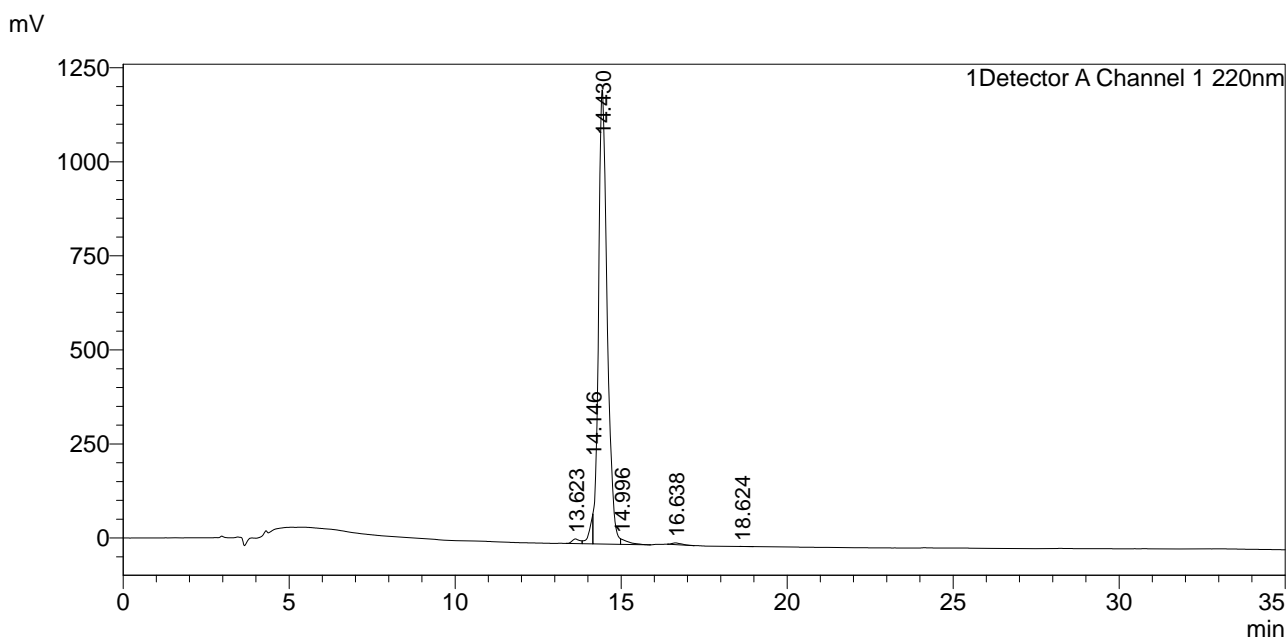

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.623	200530	12552	0.873
2	14.146	563303	75579	2.453
3	14.430	21879039	1207491	95.257
4	14.996	234426	14617	1.021
5	16.638	90017	4536	0.392
6	18.624	1156	74	0.005
Total		22968471	1314848	100.000