

Sample Name :Angiotensin I, human
 Cat No. :RP11251
 Lot No. :E2662920L
 Time Processed :8:04:59
 Month-Day-Year Processed :12/30/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

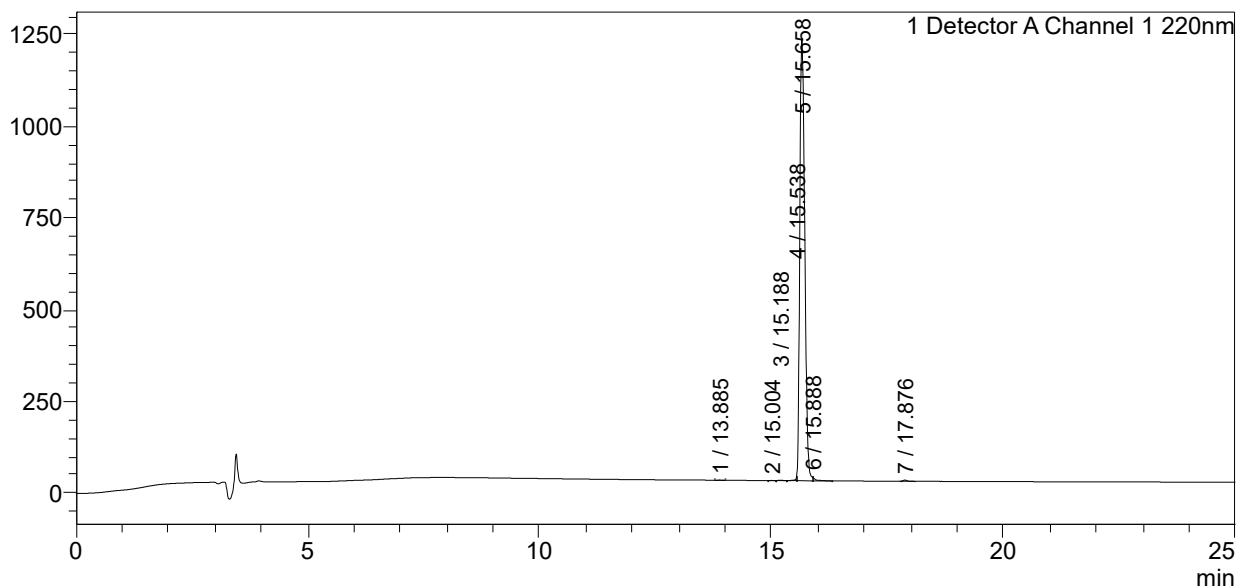

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	13.885	2828	480	0.031
2	15.004	2824	525	0.031
3	15.188	9142	1022	0.101
4	15.538	21802	5660	0.241
5	15.658	8949664	1206441	98.895
6	15.888	44933	9941	0.497
7	17.876	18424	3187	0.204
Total		9049617	1227257	100.000