

Sample Name : Atrial Natriuretic Peptide (ANP) (1-28), rat
 Cat No. :RP11195
 Lot No. :E4709820K
 Time Processed : 4:13:10 PM
 Month-Day-Year Processed : 11/14/2020


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
32.00	Pumps	Pump A B.Conc	95
32.01	Pumps	Pump A B.Conc	5
40.00	Pumps	Pump A B.Conc	5
45.00	Controller	Stop	

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: GK11010017

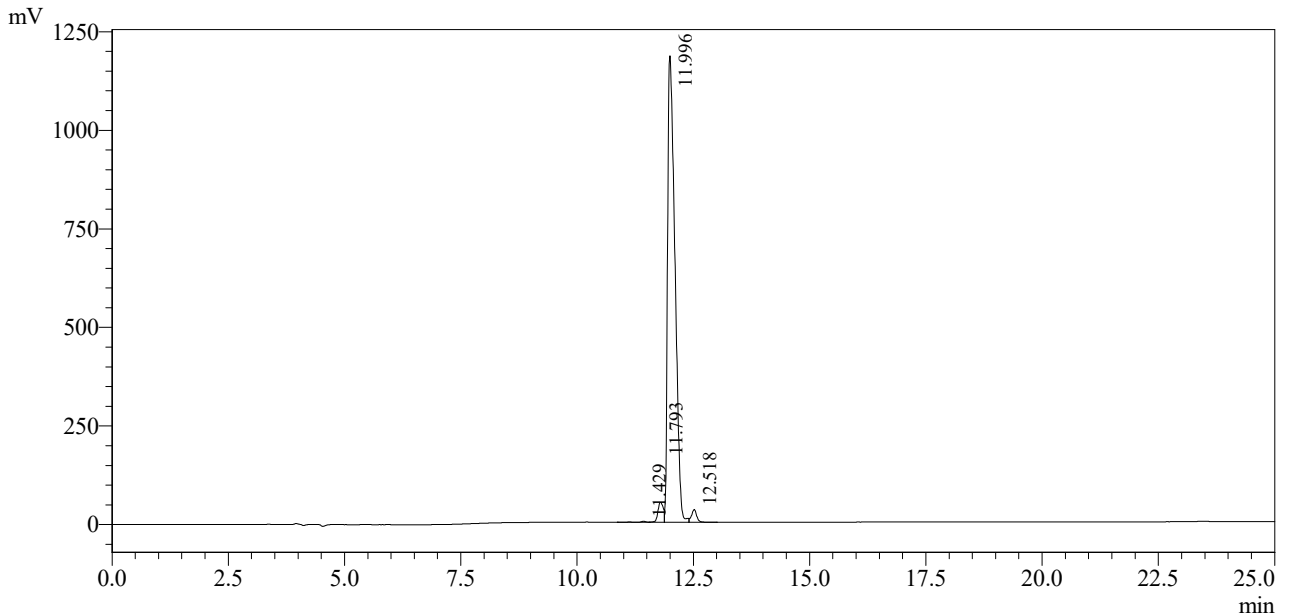

1 Detector A Channel 1 / 220nm

Peak Table

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	11.429	25298	2723	0.185
2	11.793	407337	50735	2.972
3	11.996	13023173	1182656	95.024
4	12.518	249394	32597	1.820
Total		13705201	1268711	100.000