

Sample Name :OVA G4 peptide
 Cat No. :RP20398
 Lot No. :E9204620I
 Time Processed :10:42:05 PM
 Month-Day-Year Processed :10/02/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

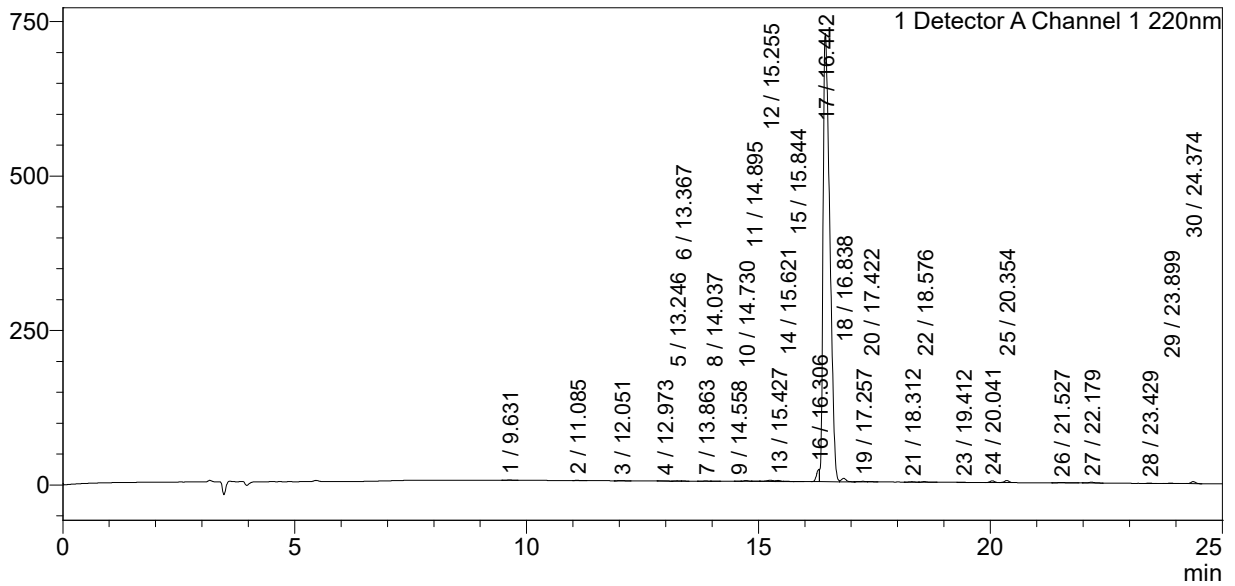

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.631	5046	563	0.066
2	11.085	2180	314	0.029
3	12.051	4156	539	0.054
4	12.973	1902	280	0.025
5	13.246	3903	607	0.051
6	13.367	1045	211	0.014
7	13.863	3538	423	0.046
8	14.037	1248	174	0.016
9	14.558	1125	198	0.015
10	14.730	8591	1336	0.113
11	14.895	1442	251	0.019
12	15.255	19740	1793	0.259
13	15.427	11576	1702	0.152
14	15.621	3519	574	0.046

Peak#	Ret. Time	Area	Height	Area%
15	15.844	1038	140	0.014
16	16.306	90359	19863	1.184
17	16.442	7321630	725319	95.919
18	16.838	37512	5637	0.491
19	17.257	6652	826	0.087
20	17.422	3063	420	0.040
21	18.312	4966	736	0.065
22	18.576	6912	1052	0.091
23	19.412	1926	269	0.025
24	20.041	18898	2822	0.248
25	20.354	23732	3513	0.311
26	21.527	9196	687	0.120
27	22.179	11683	1355	0.153
28	23.429	1776	282	0.023
29	23.899	3304	357	0.043
30	24.374	21454	3245	0.281
Total		7633114	775489	100.000