

Sample Name :CEF1, Influenza Matrix Protein M1 (58 - 66)
 Cat No. :RP19978
 Lot No. :E7319521C
 Time Processed :7:20:05 AM
 Month-Day-Year Processed :03/20/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

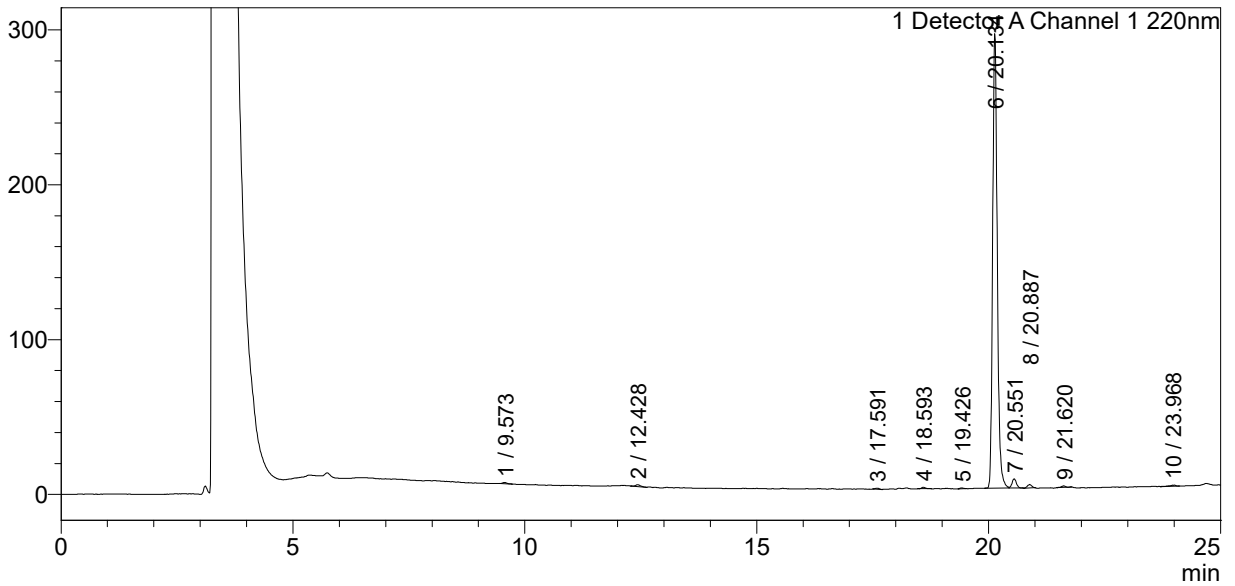

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	9.573	5066	790	0.238
2	12.428	8855	1180	0.416
3	17.591	3751	603	0.176
4	18.593	5368	981	0.252
5	19.426	2641	502	0.124
6	20.134	2037901	293637	95.769
7	20.551	39413	5998	1.852
8	20.887	13952	2117	0.656
9	21.620	4279	899	0.201
10	23.968	6713	670	0.315
Total		2127940	307377	100.000