

Sample Name: LH-RH, salmon  
 Cat No. : RP10673  
 Lot No. : E4761819I  
 Time Processed: 11:24:00 AM  
 Month-Day-Year  
 Processed :09/18/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.00	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm  
 Equipment:ZJ19010325

<Chromatogram>

mV

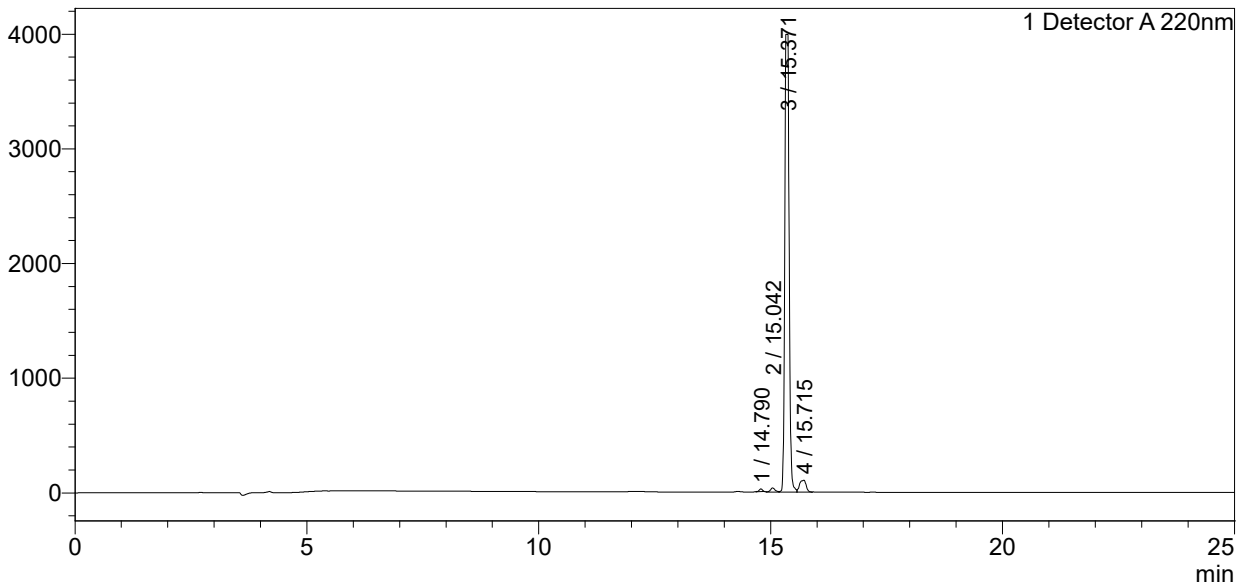

<Peak Table>

Detector A 220nm

Peak#	Ret. Time	Area	Height	Area%
1	14.790	108449	22607	0.396
2	15.042	251257	37023	0.916
3	15.371	26074241	3991971	95.104
4	15.715	982694	102196	3.584
Total		27416642	4153796	100.000