

Sample Name :p2Ca
 Cat No. :RP19988
 Lot No. :E4830019I
 Time Processed :6:08:55
 Month-Day-Year Processed :09/19/19

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ17010508

<Chromatogram>

mV

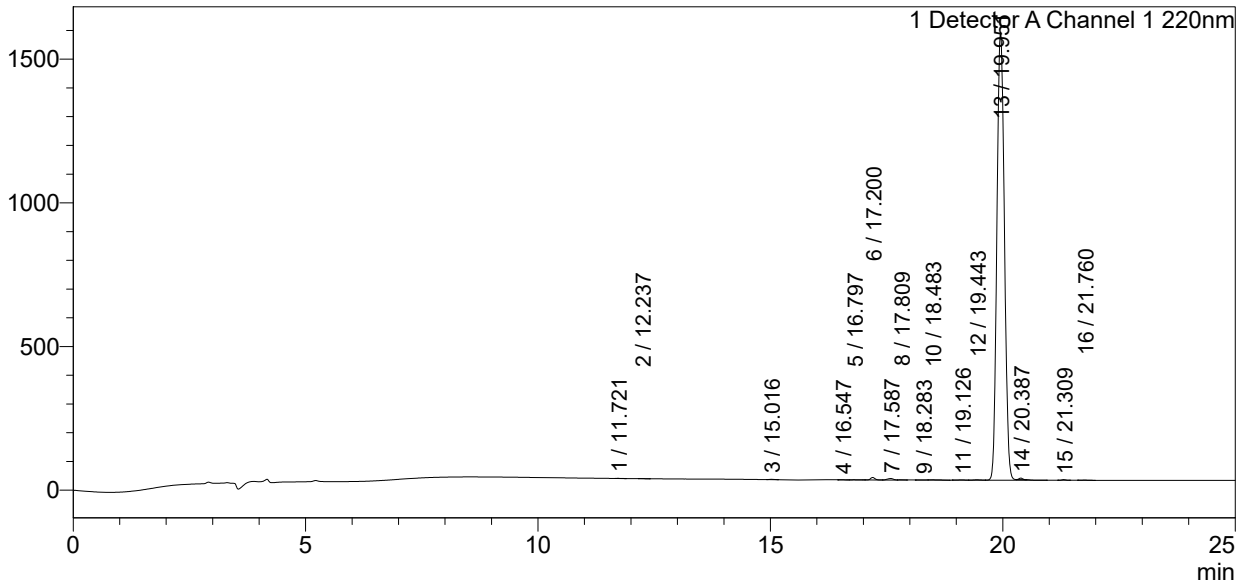

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.721	1846	390	0.010
2	12.237	2047	372	0.012
3	15.016	5240	931	0.030
4	16.547	2919	496	0.017
5	16.797	3425	496	0.019
6	17.200	57748	8827	0.326
7	17.587	46698	5223	0.264
8	17.809	8395	1481	0.047
9	18.283	7512	673	0.042
10	18.483	17401	1058	0.098
11	19.126	9538	769	0.054
12	19.443	16941	1469	0.096
13	19.951	17462842	1558350	98.705
14	20.387	29040	5461	0.164
15	21.309	13278	2243	0.075

Peak#	Ret. Time	Area	Height	Area%
16	21.760	7054	627	0.040
Total		17691924	1588866	100.000