

Sample Name :Gastric Inhibitory Peptide (GIP), human
 Cat No. :RP10795
 Lot No. :E7798121E
 Time Processed :20:31:46
 Month-Day-Year Processed :05/08/2021

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	B.Conc	5
25.00	Pumps	B.Conc	65
25.01	Pumps	B.Conc	95
27.00	Pumps	B.Conc	95
27.01	Pumps	B.Conc	5
35.00	Pumps	B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm
 Equipment: ZJ19010141

<Chromatogram>

mV

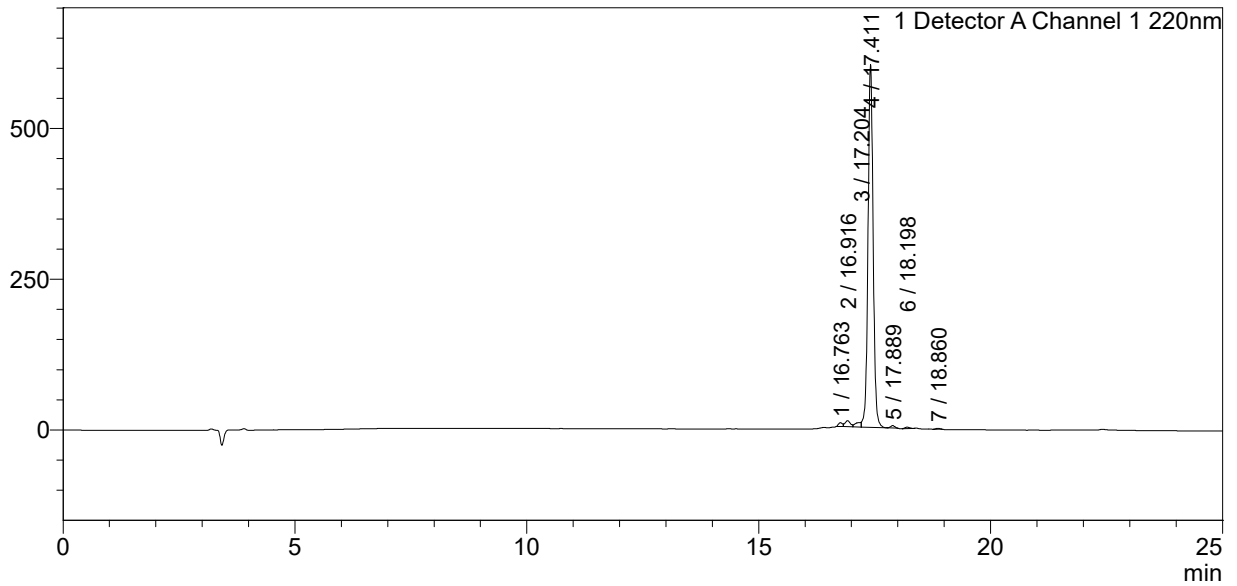

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	16.763	39198	6248	0.804
2	16.916	81807	10140	1.677
3	17.204	65182	7682	1.336
4	17.411	4644923	601983	95.218
5	17.889	23742	3939	0.487
6	18.198	15490	2252	0.318
7	18.860	7872	1468	0.161
Total		4878216	633711	100.000