

Sample Name:Endothelin 1, human, porcine
 Cat No. :RP12758 Lot No.:PE1571801


Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

| Time | Unit | Command | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01 | Pumps | Pump A B.Conc | 5 | |
| 25.00 | Pumps | Pump A B.Conc | 65 | |
| 25.01 | Pumps | Pump A B.Conc | 95 | |
| 31.00 | Pumps | Pump A B.Conc | 95 | |
| 31.01 | Pumps | Pump A B.Conc | 5 | |
| 40.00 | Pumps | Pump A B.Conc | 5 | |
| 40.01 | Controller | Stop | | |

<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

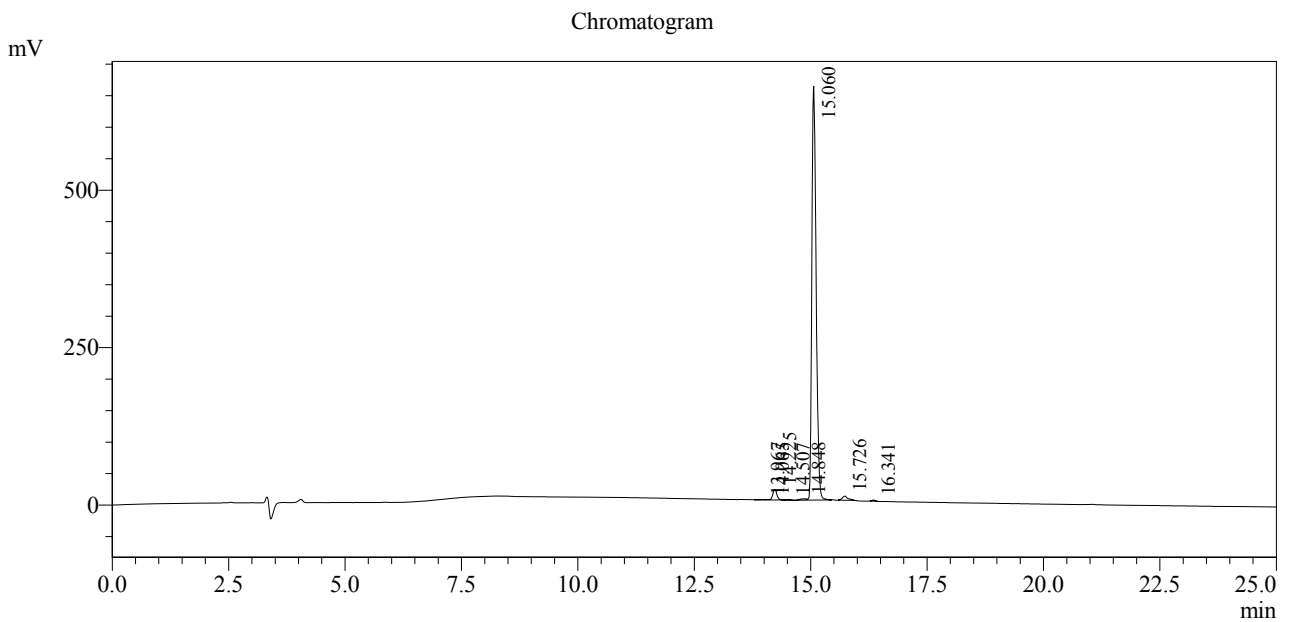

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|--------|---------|
| 1 | 13.967 | 4709 | 709 | 0.107 |
| 2 | 14.065 | 2793 | 604 | 0.063 |
| 3 | 14.225 | 100177 | 16686 | 2.266 |
| 4 | 14.507 | 3222 | 505 | 0.073 |
| 5 | 14.848 | 21620 | 2327 | 0.489 |
| 6 | 15.060 | 4223126 | 657062 | 95.519 |
| 7 | 15.726 | 57499 | 6613 | 1.301 |
| 8 | 16.341 | 8078 | 1785 | 0.183 |
| Total | | 4421224 | 686290 | 100.000 |