

Sample Name :PAR-4 Agonist Peptide, amide  
 Cat. No. : RP11529  
 Lot. No. : E5918519K  
 Time Processed :8:10:32  
 Month-Day-Year Processed : 11/16/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
27.00	Pumps	Pump A B.Conc	95	
27.01	Pumps	Pump A B.Conc	5	
35.00	Pumps	Pump A B.Conc	5	
35.00	Controller	Stop		


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0286

Chromatogram

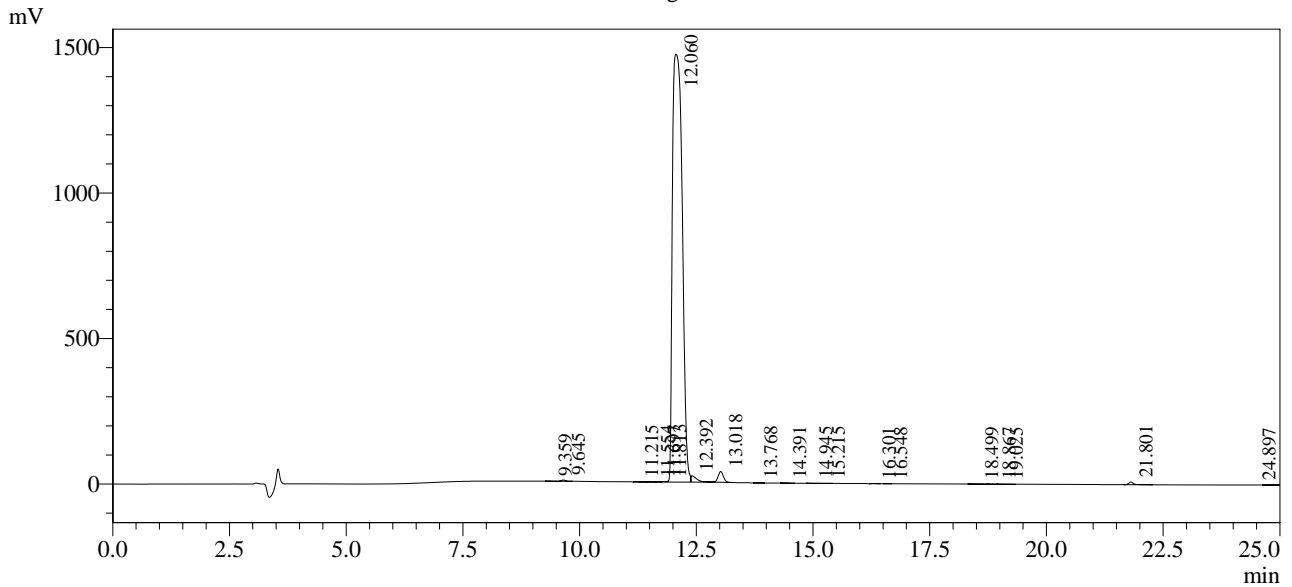

1 Det. A Ch1 / 220nm  
 Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	9.359	3323	629	0.015
2	9.645	32176	4580	0.146
3	11.215	2135	266	0.010
4	11.554	2377	369	0.011
5	11.697	5211	1013	0.024
6	11.813	12330	2230	0.056
7	12.060	21461921	1471079	97.131
8	12.392	183990	21276	0.833
9	13.018	290585	37407	1.315
10	13.768	1189	180	0.005
11	14.391	2033	274	0.009
12	14.945	1151	147	0.005
13	15.215	2434	329	0.011
14	16.301	2556	415	0.012
15	16.548	1011	187	0.005
16	18.499	7260	983	0.033
17	18.867	3602	527	0.016
18	19.025	8204	751	0.037
19	21.801	65486	9165	0.296
20	24.897	6861	602	0.031
Total		22095833	1552408	100.000