

Sample Name :MAGE-A3 (195-203)
 Cat No. :RP20413
 Lot No. :E4942519I
 Time Processed :10:30:40
 Month-Day-Year Processed :09/19/2019

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Solvent B Conc.	5
25.00	Pumps	Solvent B Conc.	65
25.01	Pumps	Solvent B Conc.	95
27.00	Pumps	Solvent B Conc.	95
27.01	Pumps	Solvent B Conc.	5
33.00	Pumps	Solvent B Conc.	5
33.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : Inertsil ODS-3 4.6 x 250 mm
 Equipment:ZJ17010507

<Chromatogram>

mV

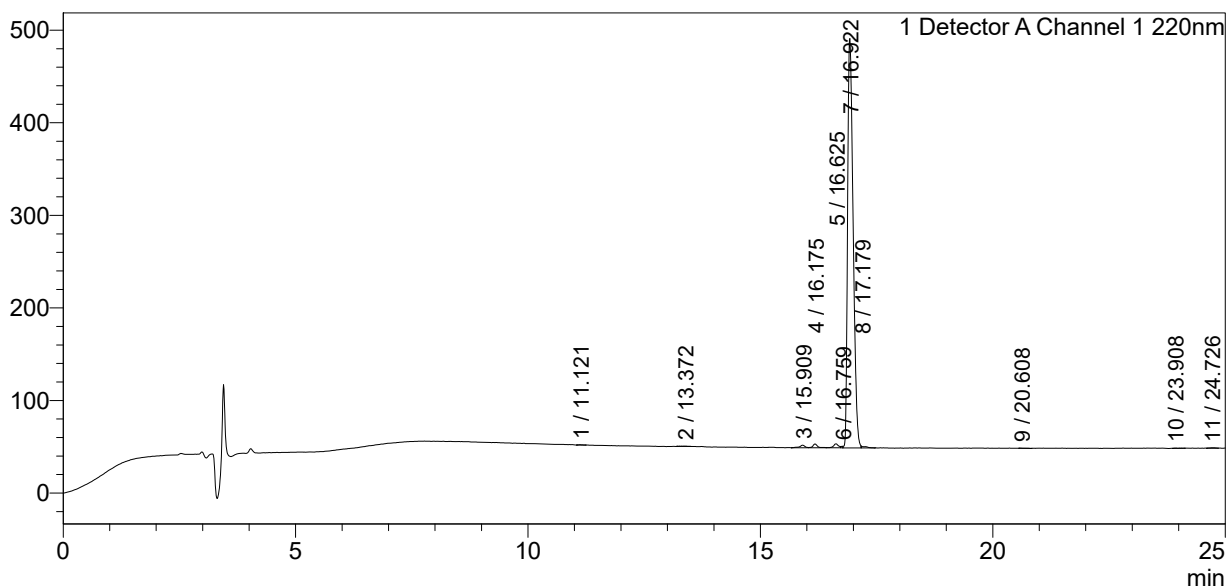

<Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	11.121	1124	247	0.030
2	13.372	4100	330	0.109
3	15.909	21896	2781	0.584
4	16.175	28785	4138	0.768
5	16.625	32233	4352	0.859
6	16.759	4659	1586	0.124
7	16.922	3635176	442190	96.932
8	17.179	13179	1767	0.351
9	20.608	1521	226	0.041
10	23.908	2194	226	0.059
11	24.726	5373	540	0.143
Total		3750241	458382	100.000