

Sample Name :Somatostatin  
Cat No.: RP10226 Lot No.: PE4961703

Pump A : 0.065% trifluoroacetic in 100% water (v/v)  
Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)  
Total Flow:1 ml/min  
Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump B Conc.	5
10.00	Pumps	Pump B Conc.	35
35.00	Pumps	Pump B Conc.	95
41.00	Pumps	Pump B Conc.	95
41.01	Pumps	Pump B Conc.	5
50.00	Pumps	Pump B Conc.	5
50.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

### <Chromatogram>

mV

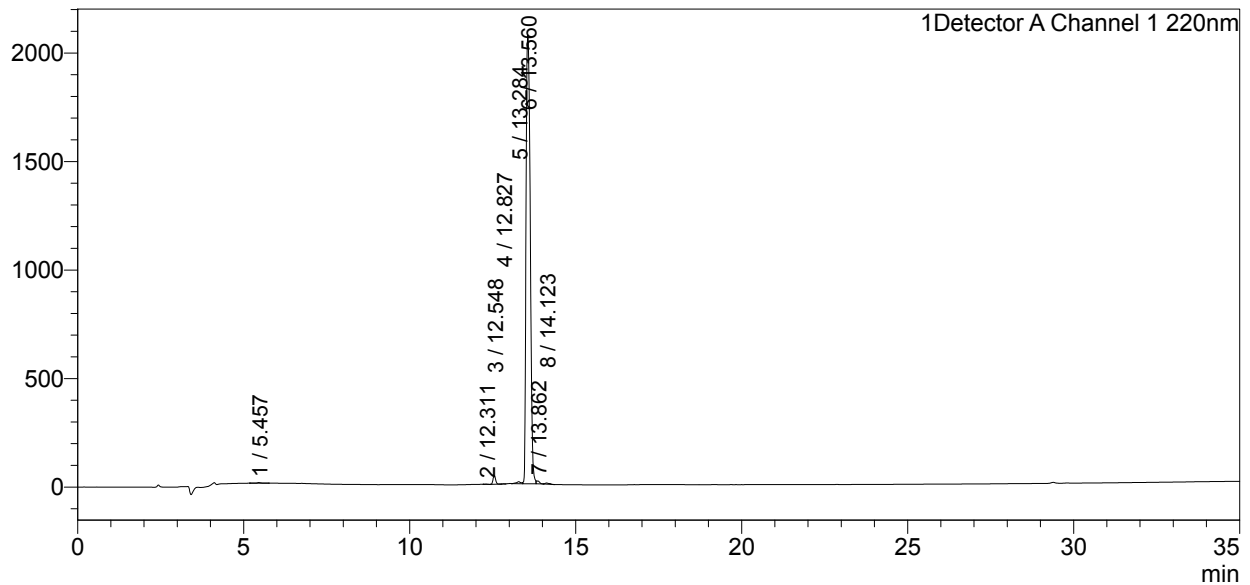

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	5.457	20187	2855	0.109
2	12.311	5613	1122	0.030
3	12.548	217646	40466	1.174
4	12.827	3053	654	0.016
5	13.284	88347	9009	0.476
6	13.560	18079748	2069065	97.491
7	13.862	84303	13276	0.455
8	14.123	46135	5041	0.249
Total		18545031	2141487	100.000