

Sample Name : HA Peptide
 Cat. No. : RP11735
 Lot. No. : E1330720A
 Time Processed : 8:06:32
 Month-Day-Year Processed : 01/03/2020

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
27.00	Pumps	Pump B Conc.	95	
27.01	Pumps	Pump B Conc.	5	
35.00	Pumps	Pump B Conc.	5	
35.01	Controller	Stop		


<<Column Performance>>

<Detector A>

Column :Inertsil ODS-3 4.6 x 250 mm

Equipment: SS-CM-0309

Chromatogram

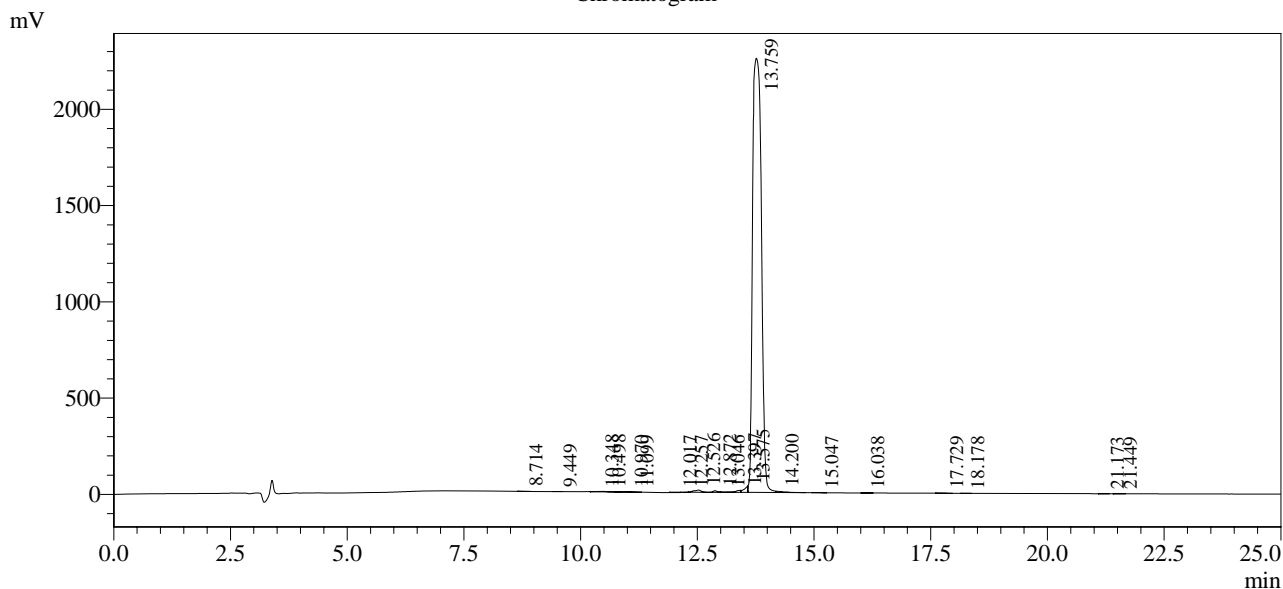

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	8.714	2307	283	0.008
2	9.449	1323	239	0.004
3	10.348	15935	2055	0.053
4	10.498	18159	2376	0.060
5	10.970	7626	920	0.025
6	11.099	3340	649	0.011
7	12.017	3211	419	0.011
8	12.257	4715	648	0.016
9	12.526	128088	11574	0.425
10	12.872	53606	8252	0.178
11	13.046	16234	2220	0.054
12	13.397	88803	10613	0.294
13	13.575	175539	32104	0.582
14	13.759	29552449	2255083	97.958
15	14.200	82608	6650	0.274
16	15.047	5225	554	0.017
17	16.038	1037	112	0.003
18	17.729	4610	481	0.015
19	18.178	1185	225	0.004
20	21.173	1089	146	0.004
21	21.449	1330	106	0.004
Total		30168419	2335709	100.000