

Sample Name :  $\beta$ -Amyloid(1-42),human  
 Cat. No. : RP20527  
 Lot No. : E18825201  
 Time Processed :6:20:42 PM  
 Month-Day-Year Processed :10/24/2020

Pump A : 0.5% Ammonia solution in 100% water (v/v)  
 Pump B : 0.2% Ammonia solution in 100% acetonitrile (v/v)  
 Total Flow:1 ml/min  
 Wavelength:220 nm

<<LC Time Program>>

Time	Module	Command	Value
0.01	Pumps	Pump A B.Conc	5
25.00	Pumps	Pump A B.Conc	65
25.01	Pumps	Pump A B.Conc	95
27.00	Pumps	Pump A B.Conc	95
27.01	Pumps	Pump A B.Conc	5
35.00	Pumps	Pump A B.Conc	5
35.01	Controller	Stop	


<<Column Performance>>

<Detector A>

Column :UniPS 10-300 4.6 x 250 mm  
 Equipment: SS-CM-0286

### <Chromatogram>

mV

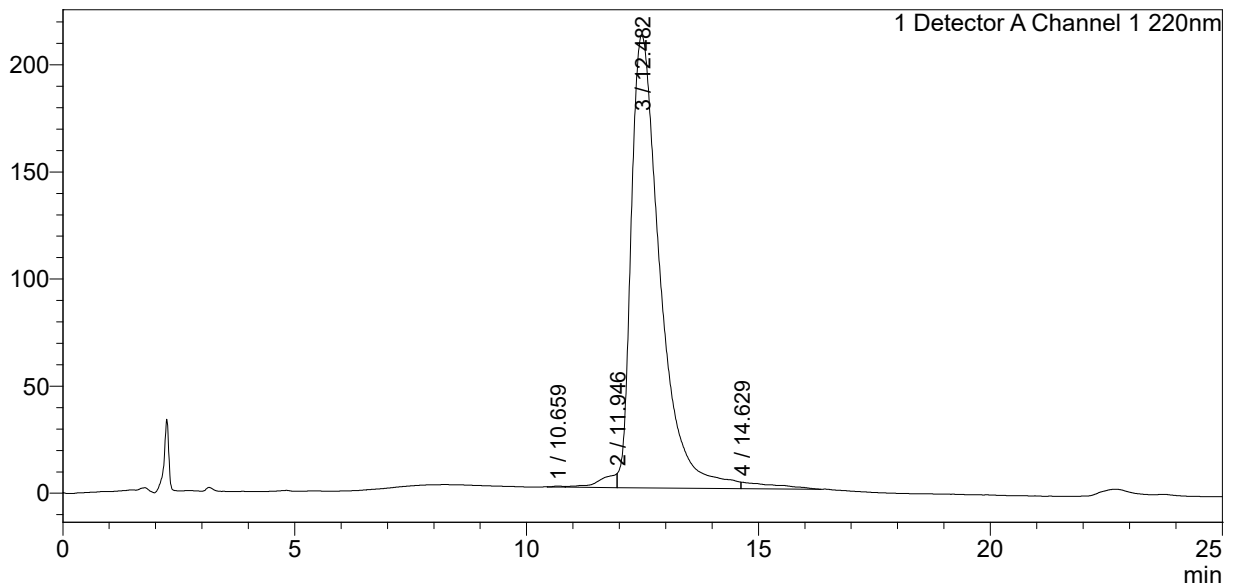

### <Peak Table>

Detector A Channel 1 220nm

Peak#	Ret. Time	Area	Height	Area%
1	10.659	7925	486	0.084
2	11.946	163657	6369	1.732
3	12.482	9123781	211137	96.574
4	14.629	152047	3020	1.609
Total		9447410	221013	100.000